

FIG. 2

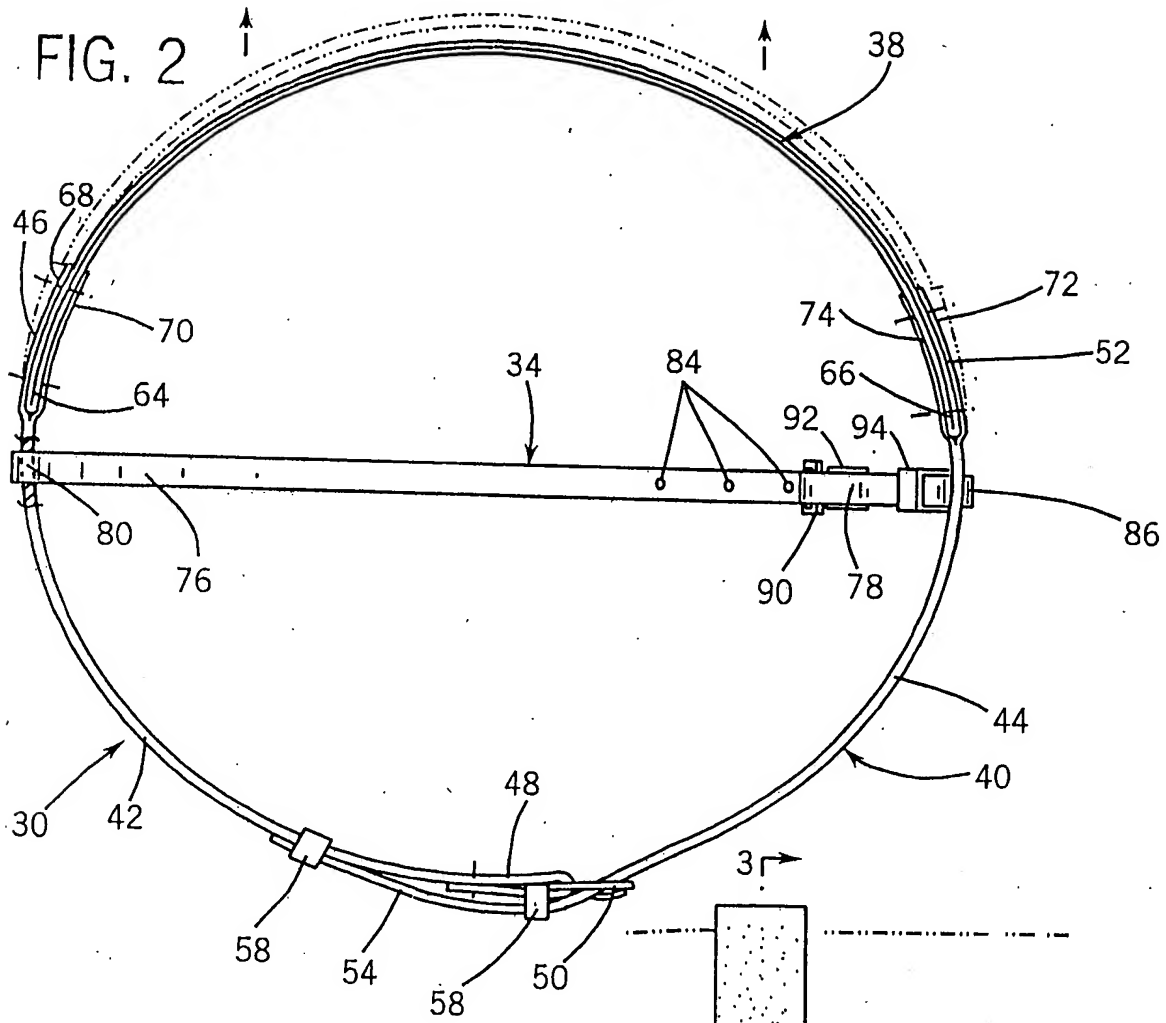


FIG. 4

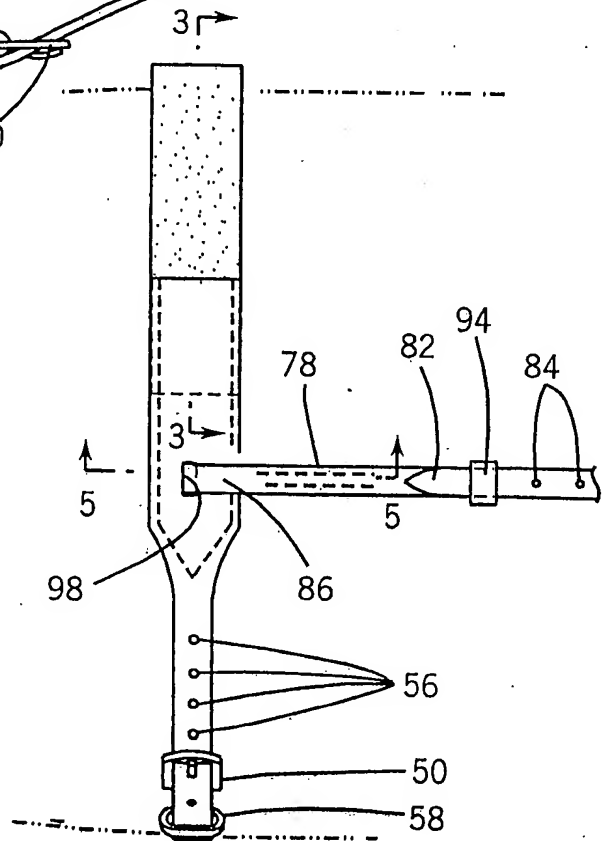
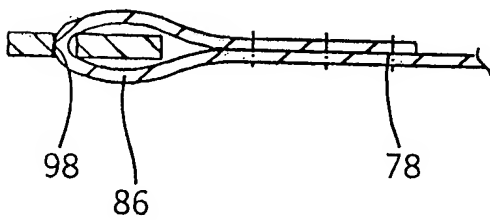


FIG. 5



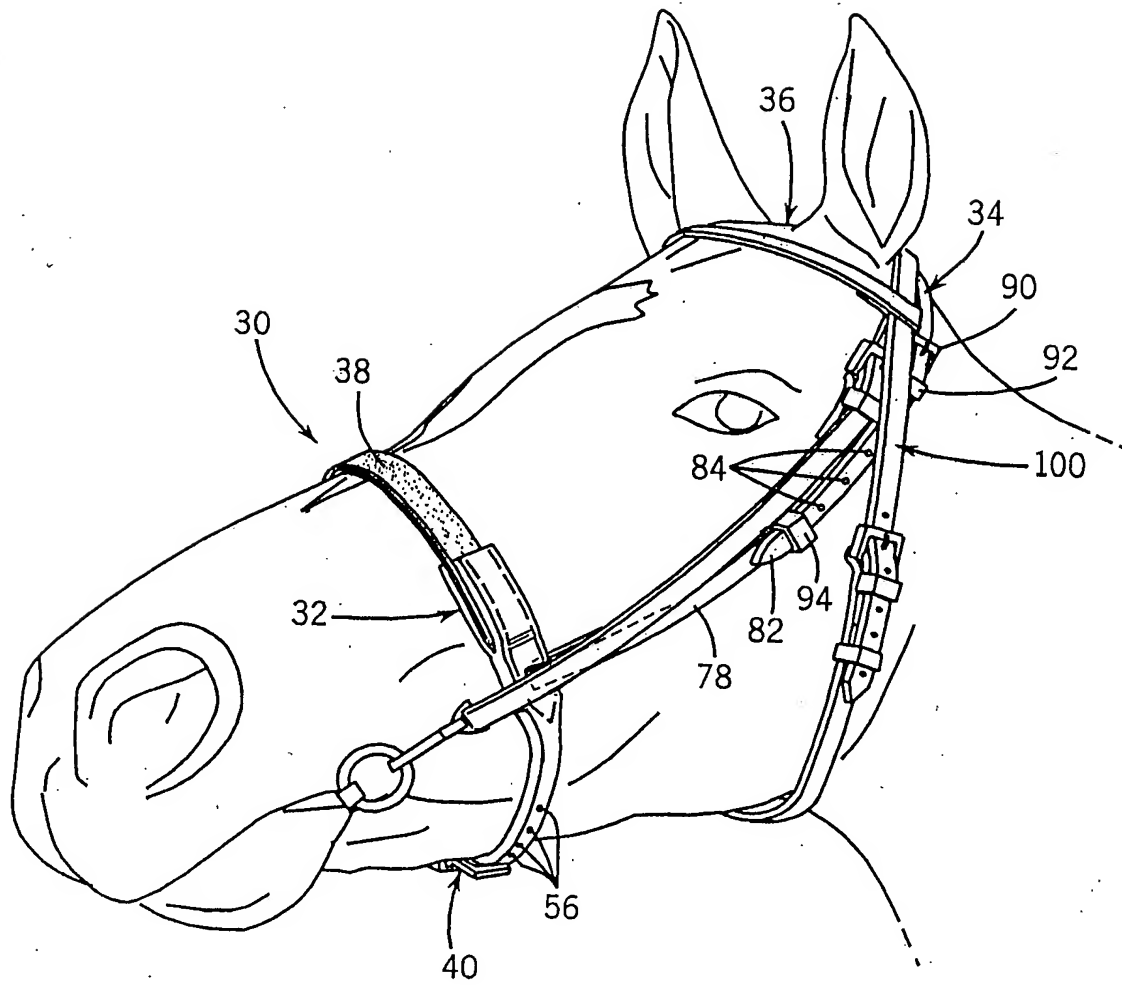


FIG. 6

4 / 36

FIG. 7

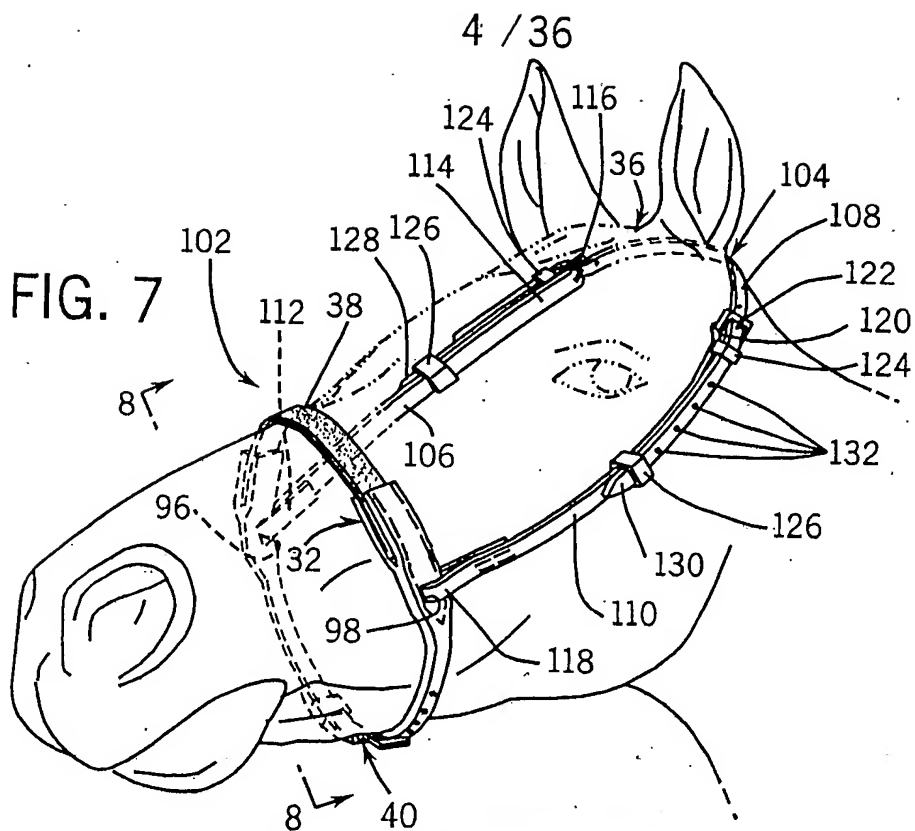


FIG. 8

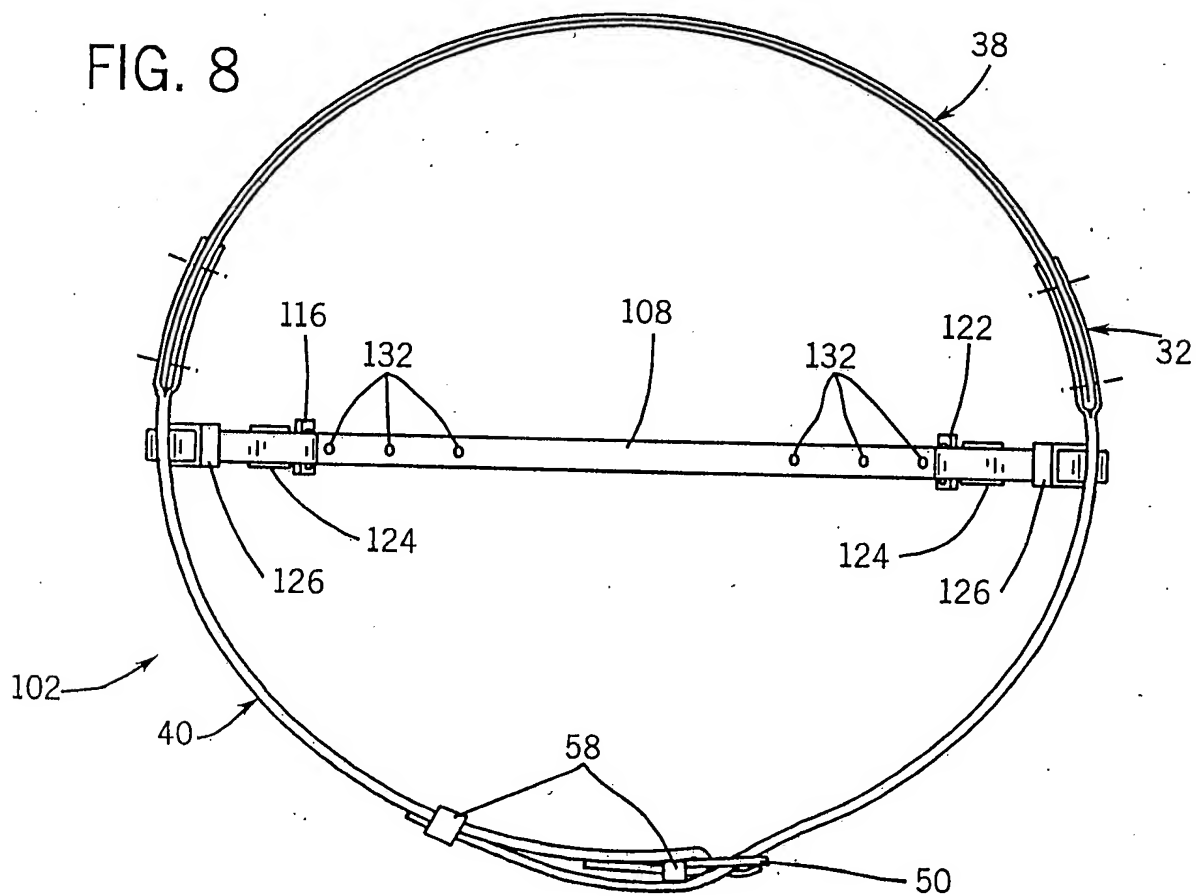


FIG. 10

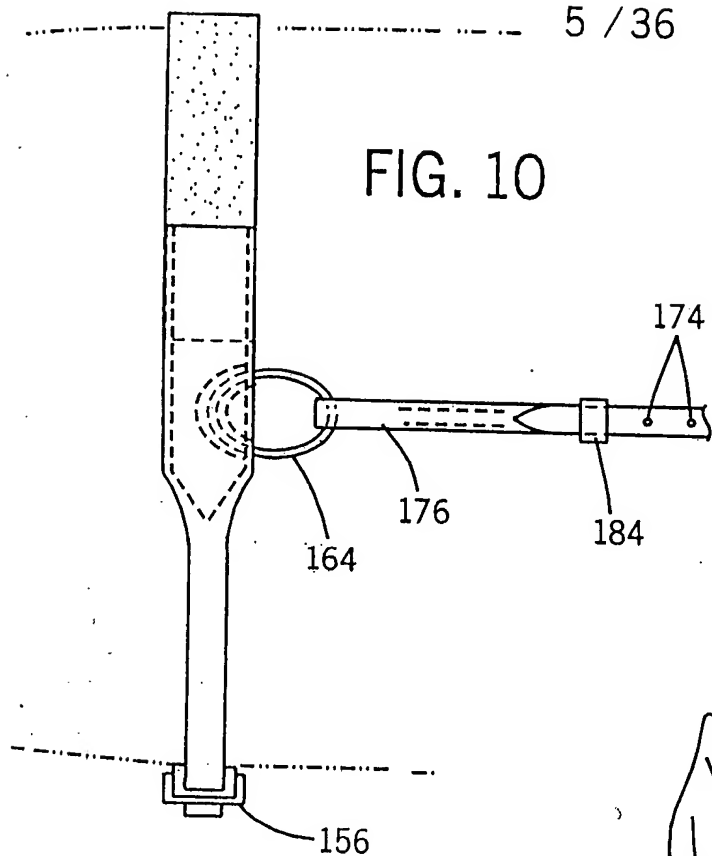


FIG. 9

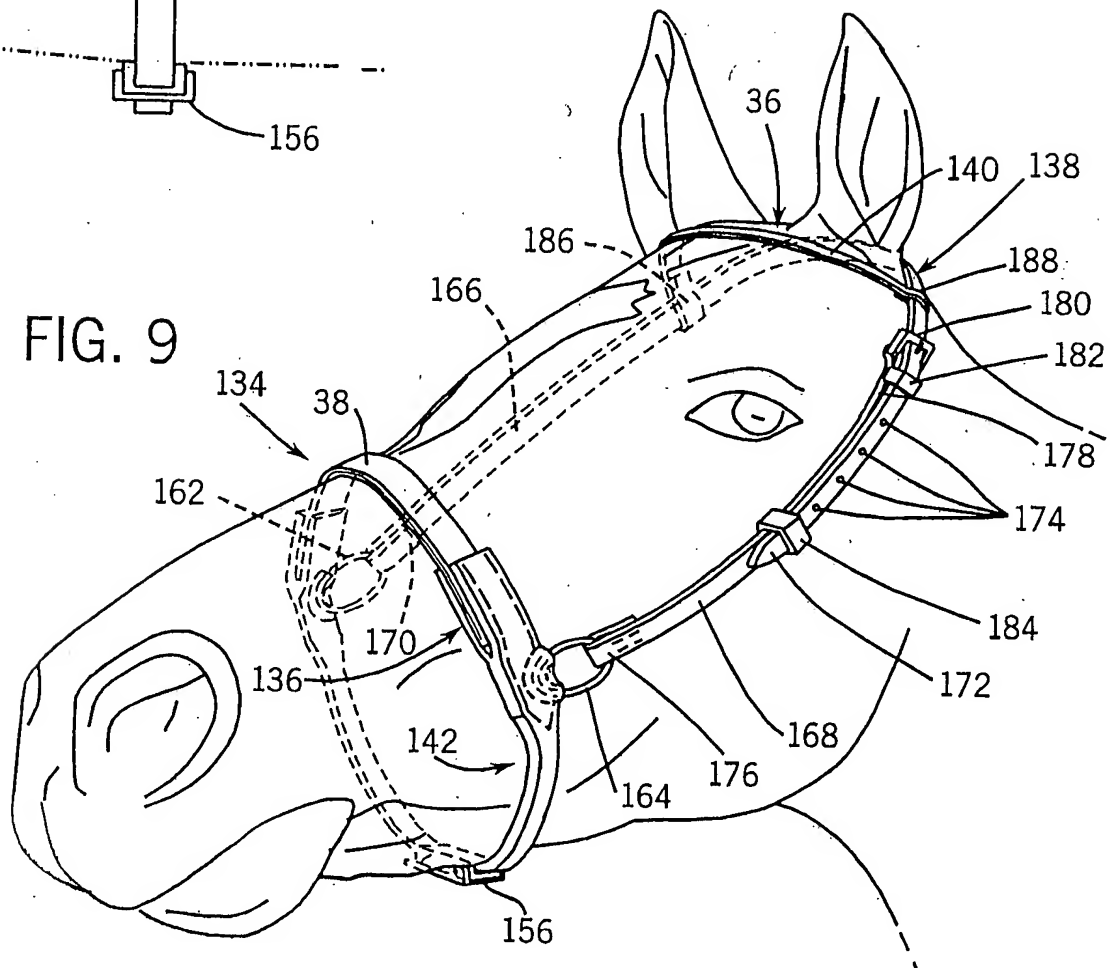


FIG. 11 is a schematic diagram of a circular device, possibly a medical device or a sensor. The device consists of a circular frame with a central horizontal bar. The frame is composed of multiple concentric layers, with the outermost layer labeled 38. The central bar is labeled 138. Various components are labeled with reference numerals: 152, 154, 64, 148, 144, 142, 146, 150, 156, 160, 162, 164, 66, 158, 174, 180, and 134. The diagram shows a cross-section of the device, with arrows indicating the direction of movement or force applied to the frame.

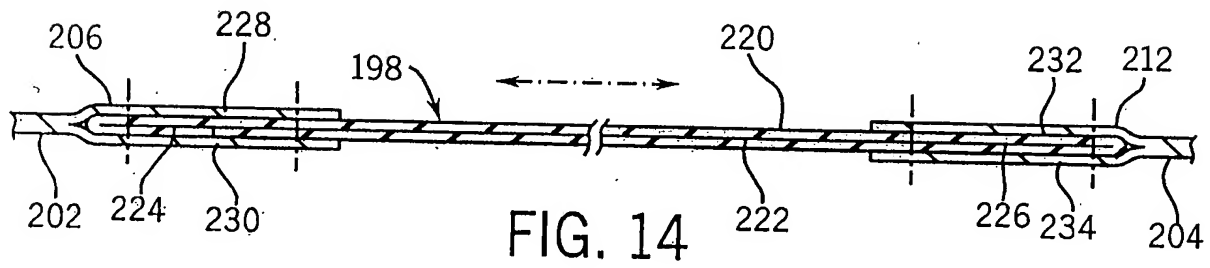
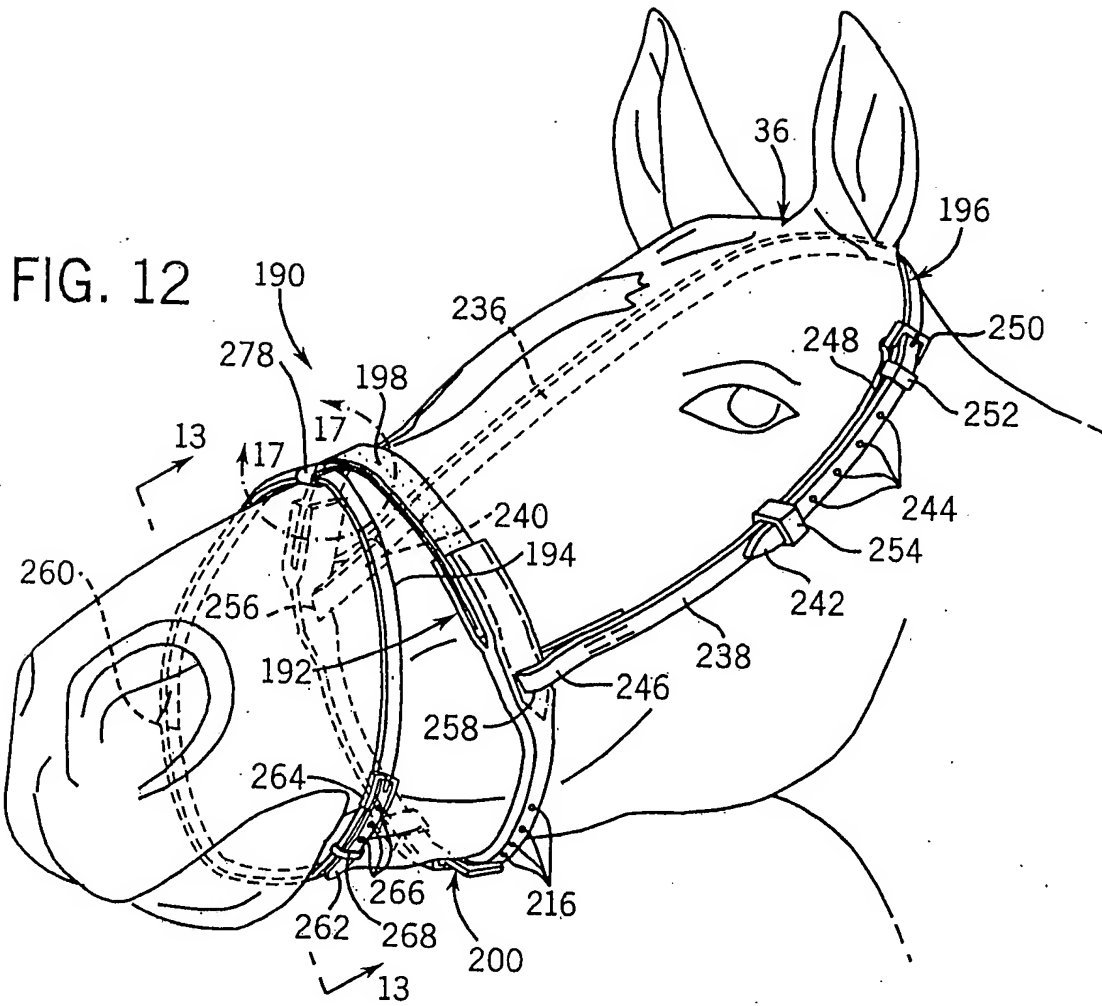


FIG. 13

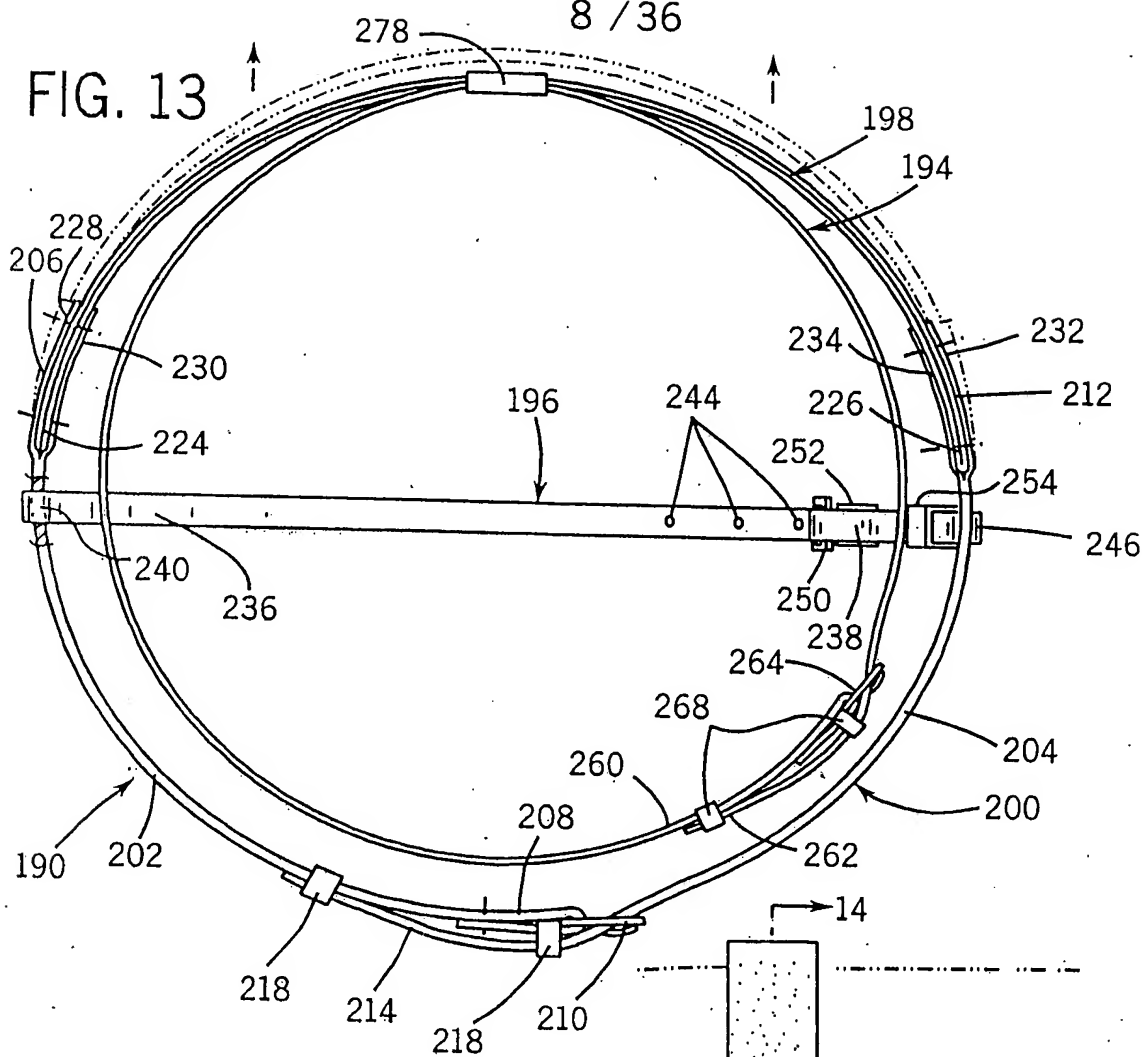


FIG. 15

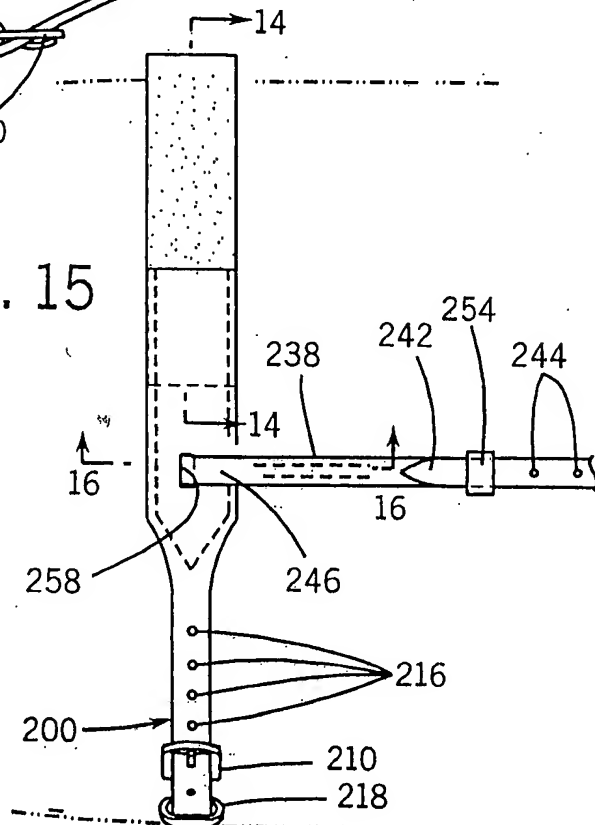


FIG. 16

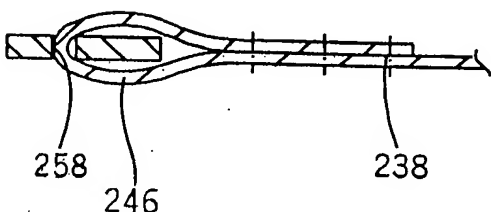




FIG. 17

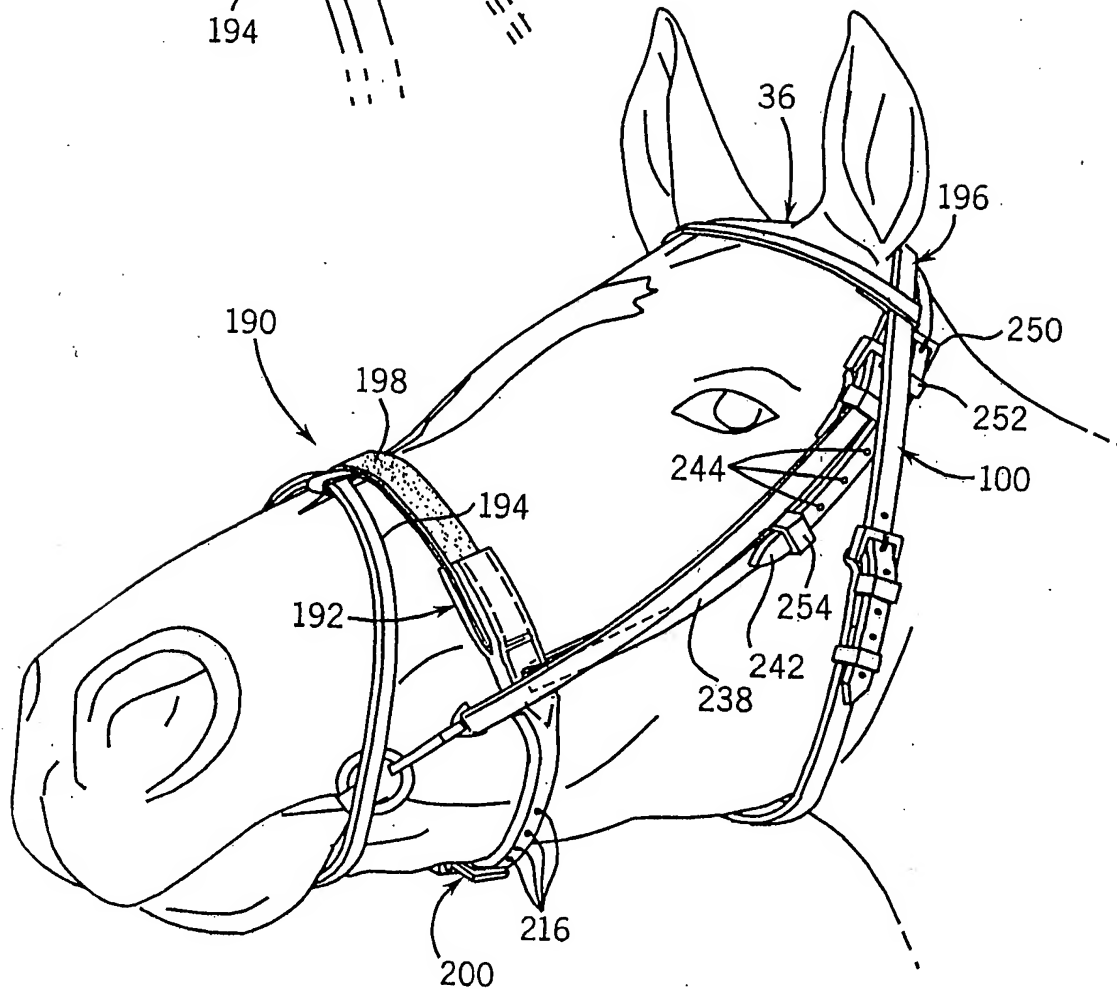
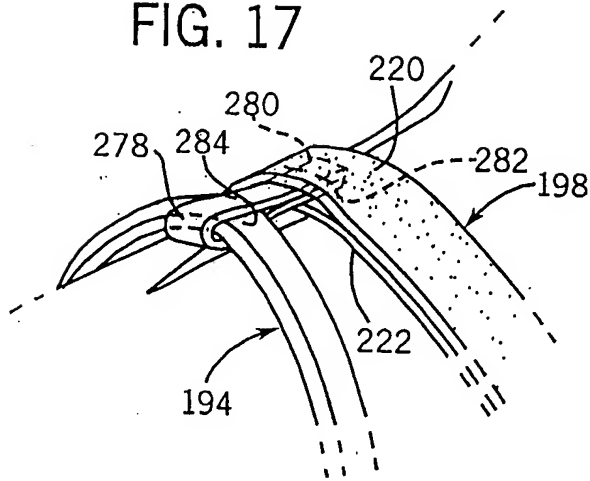
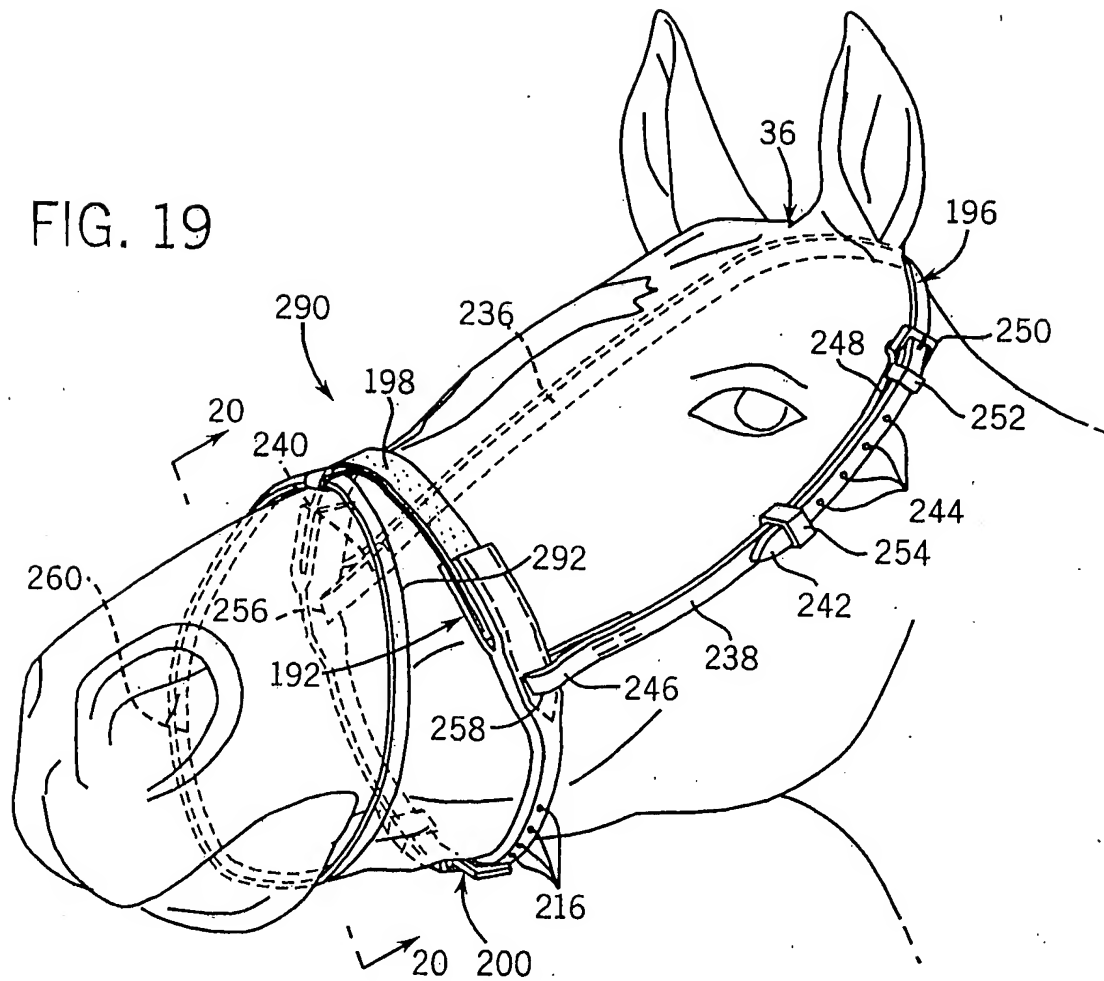


FIG. 18

FIG. 19



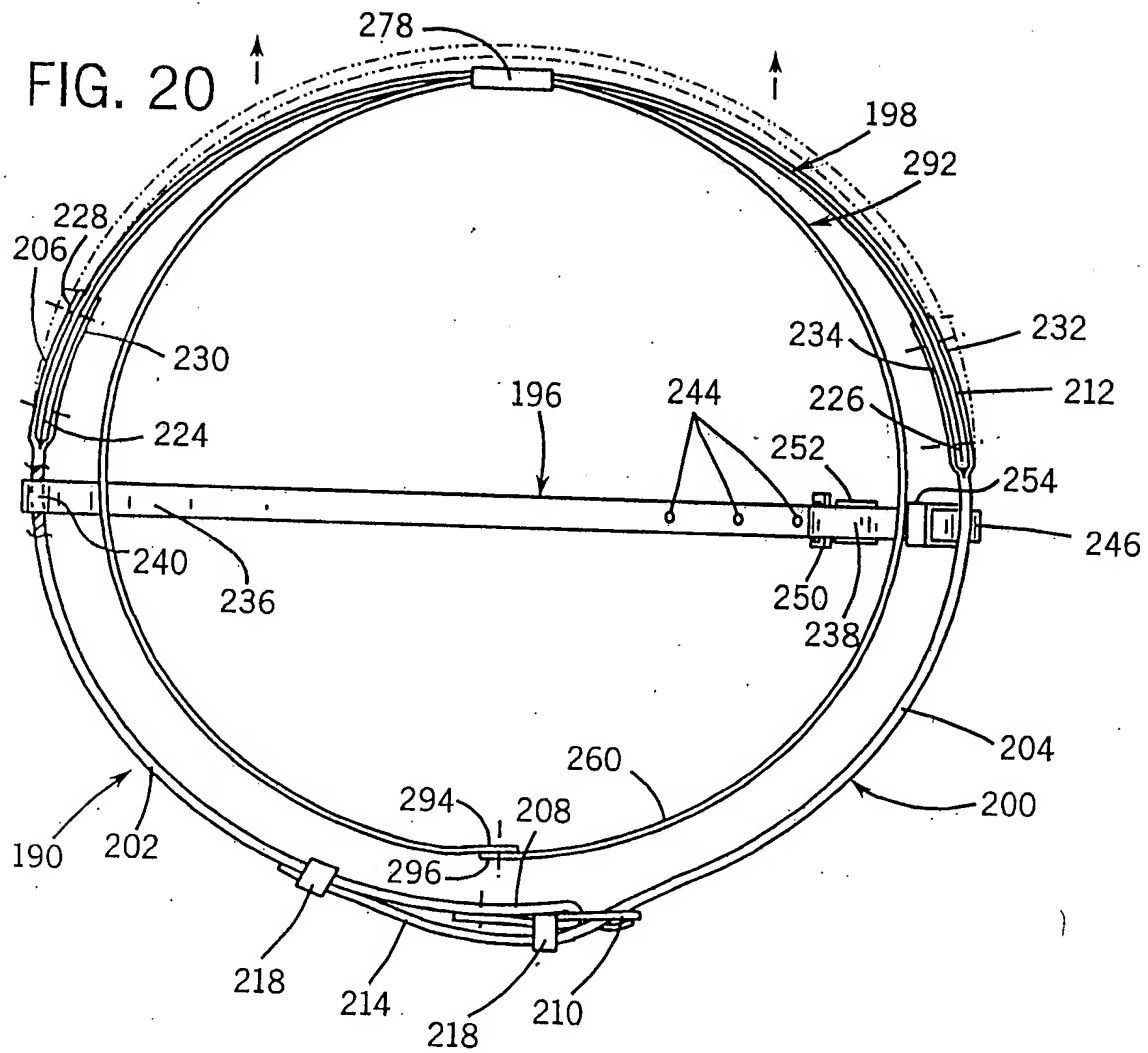


FIG. 21

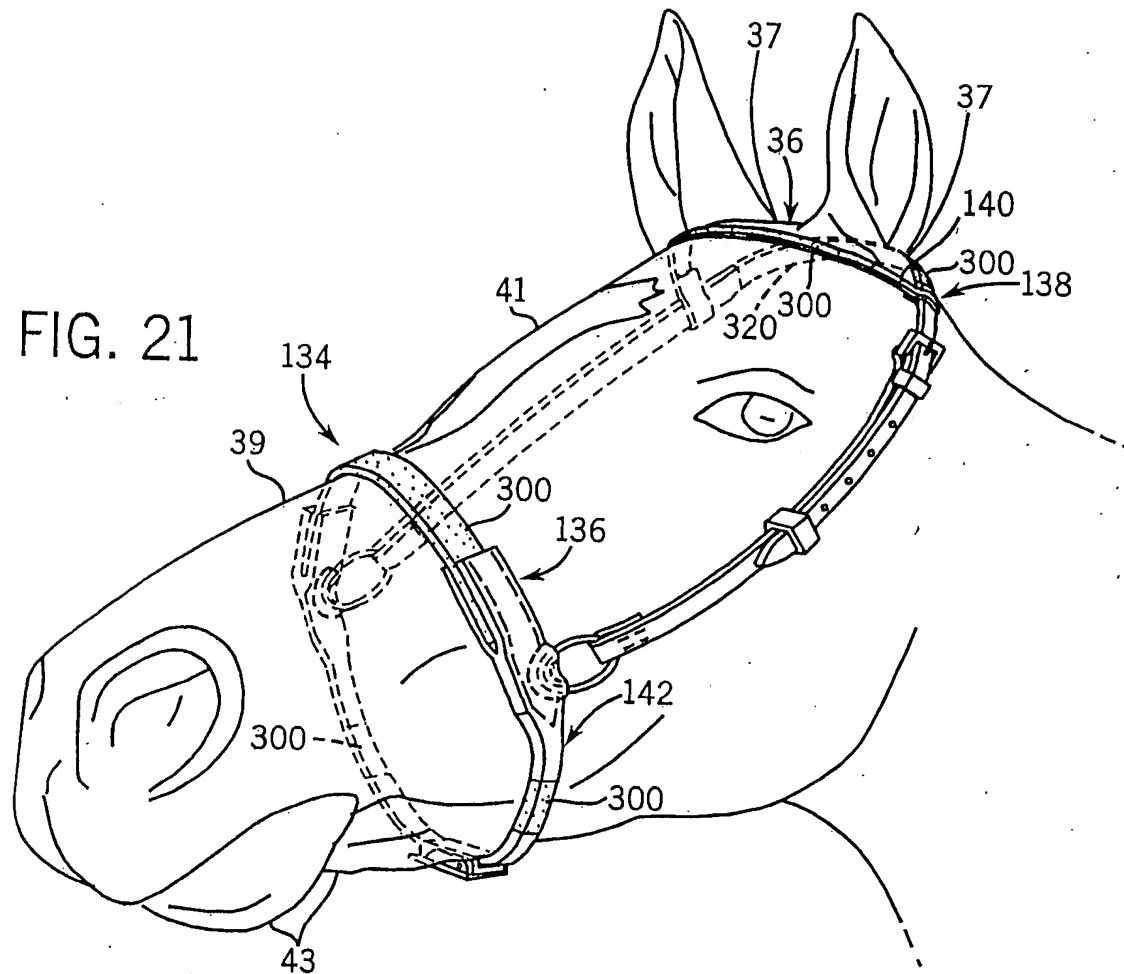
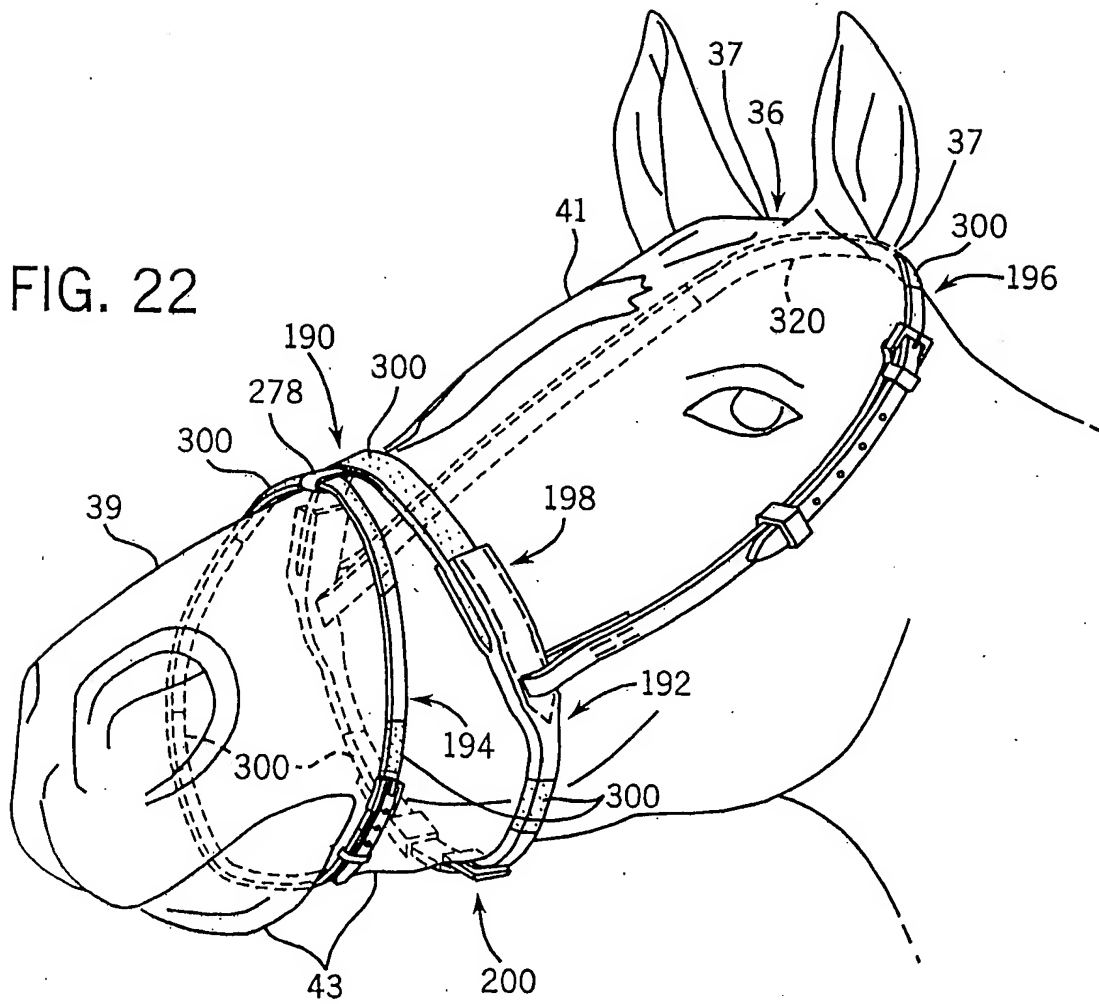


FIG. 22



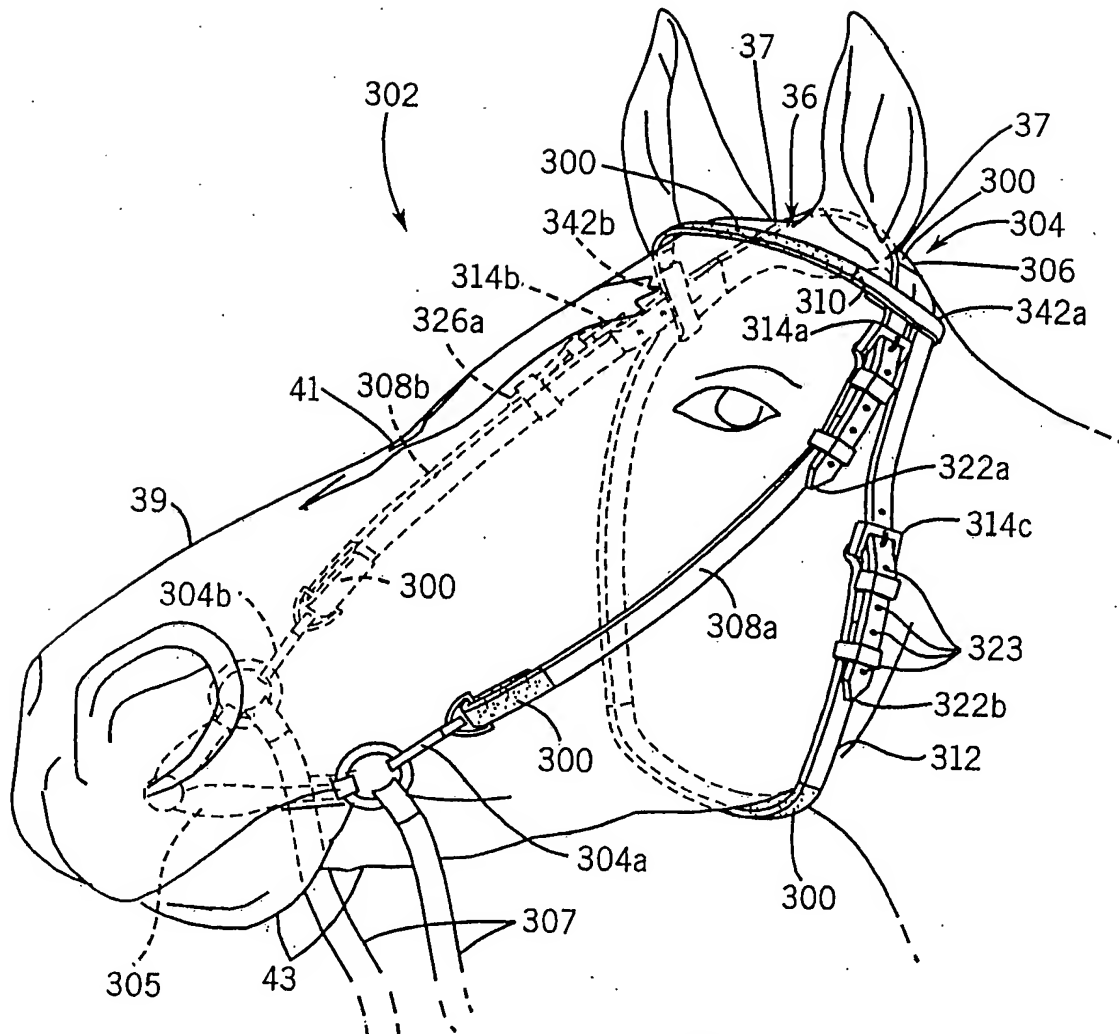


FIG. 23

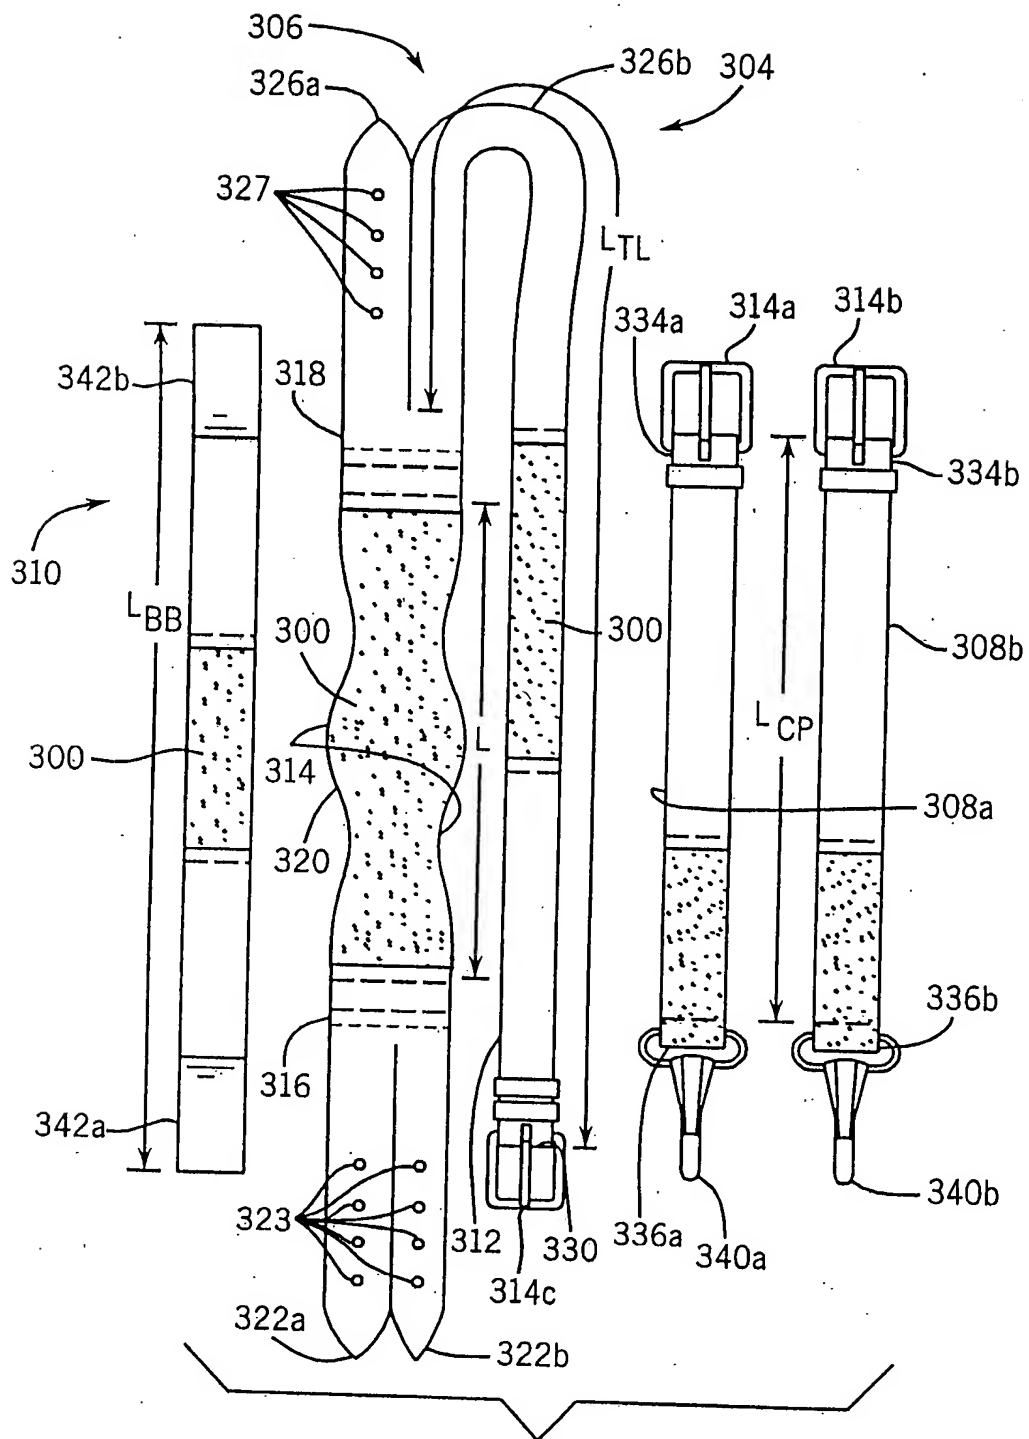
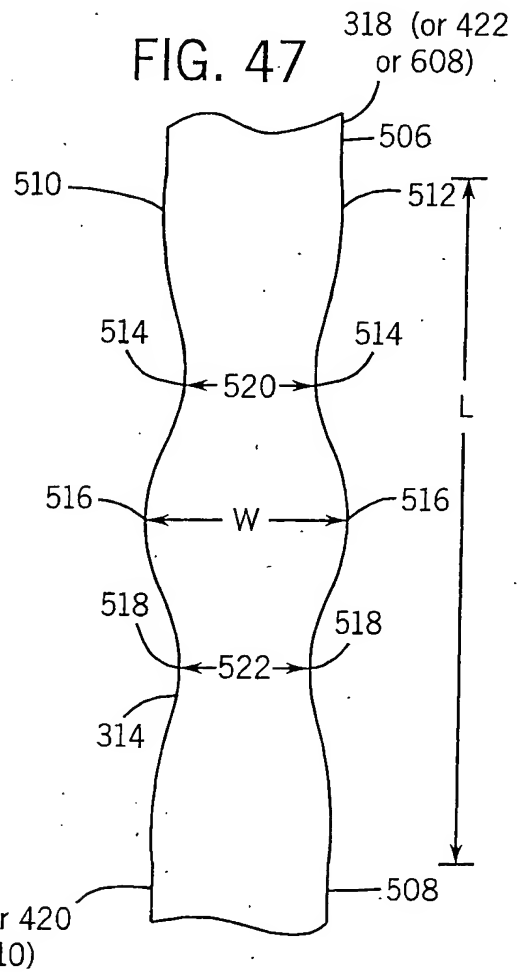
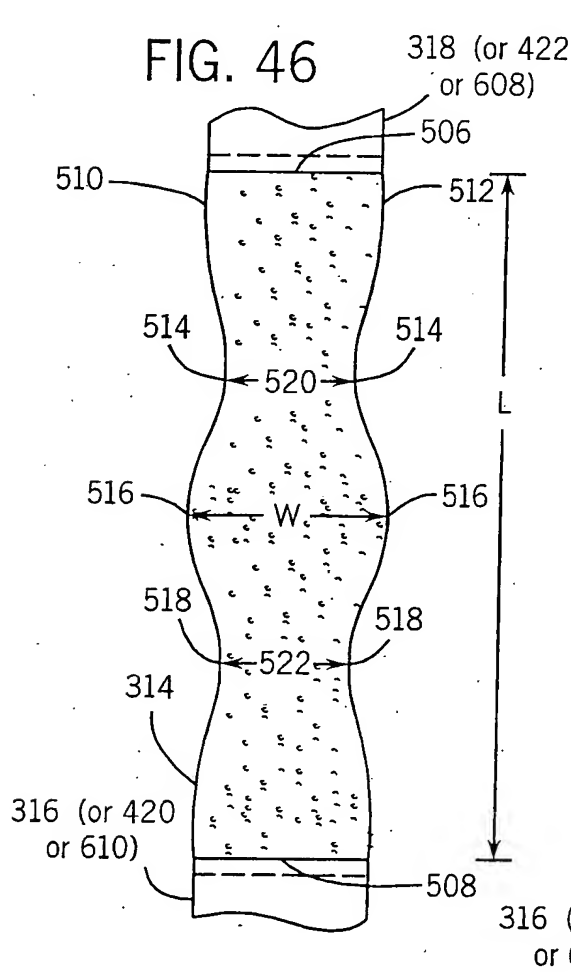
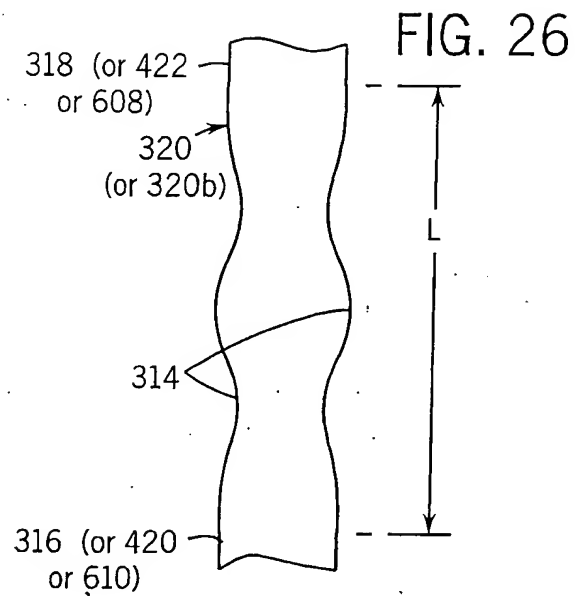
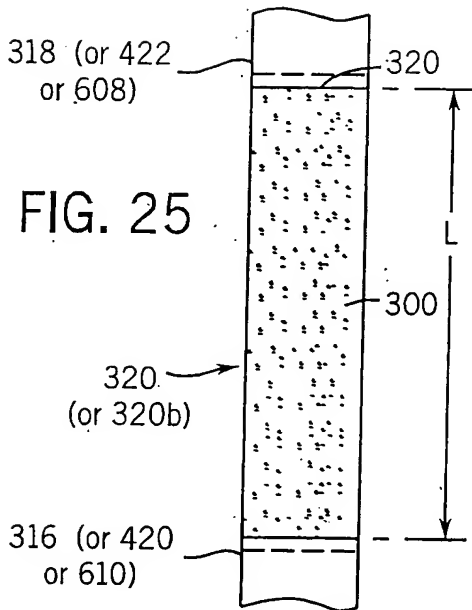
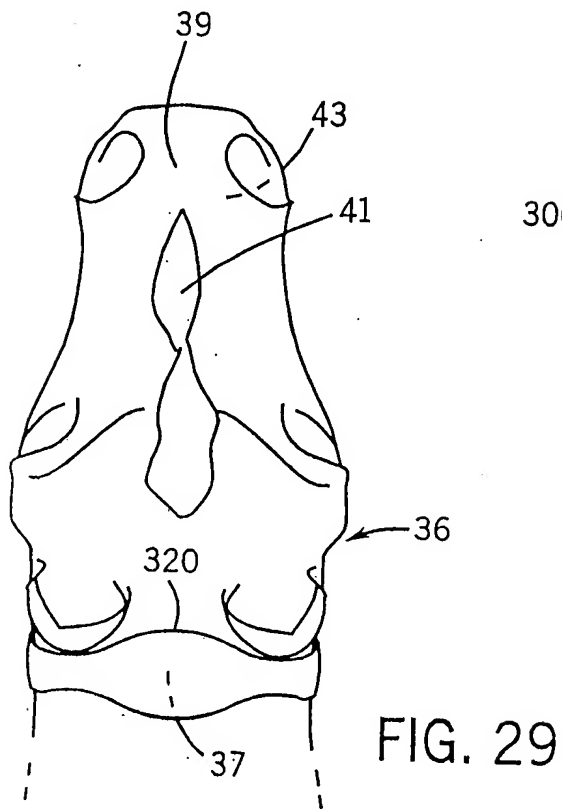
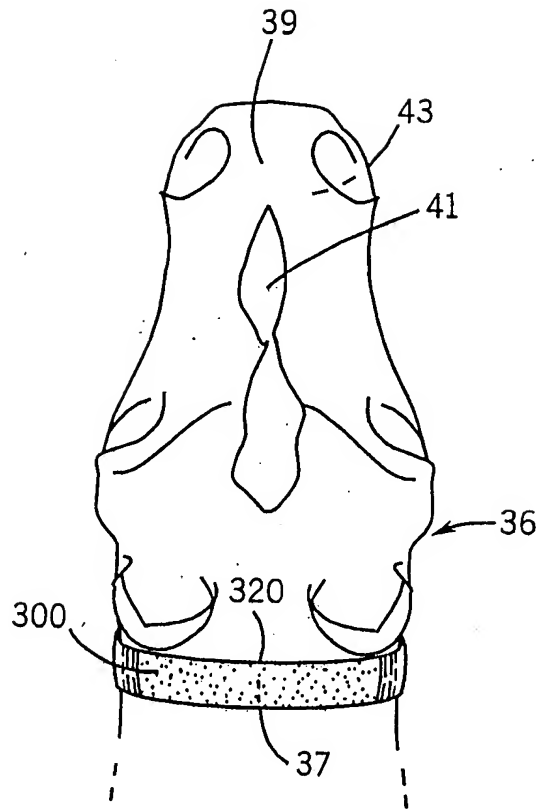
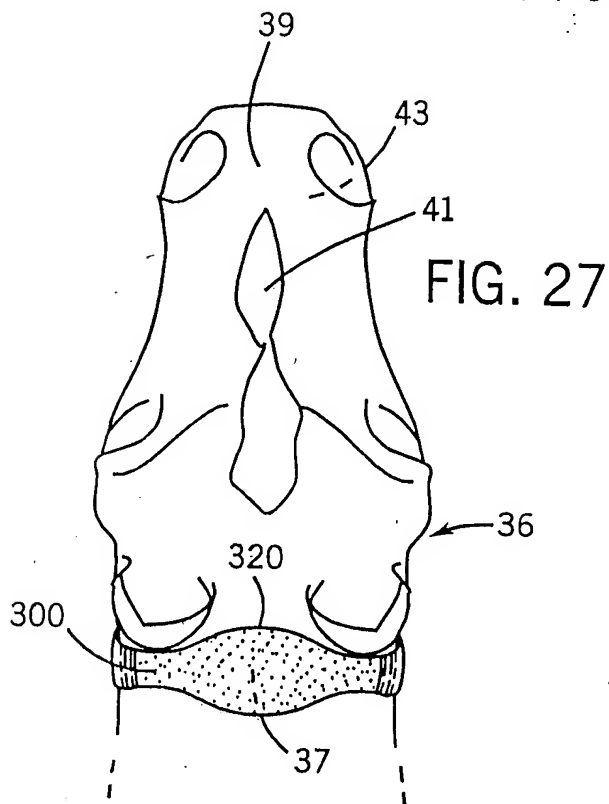


FIG. 24







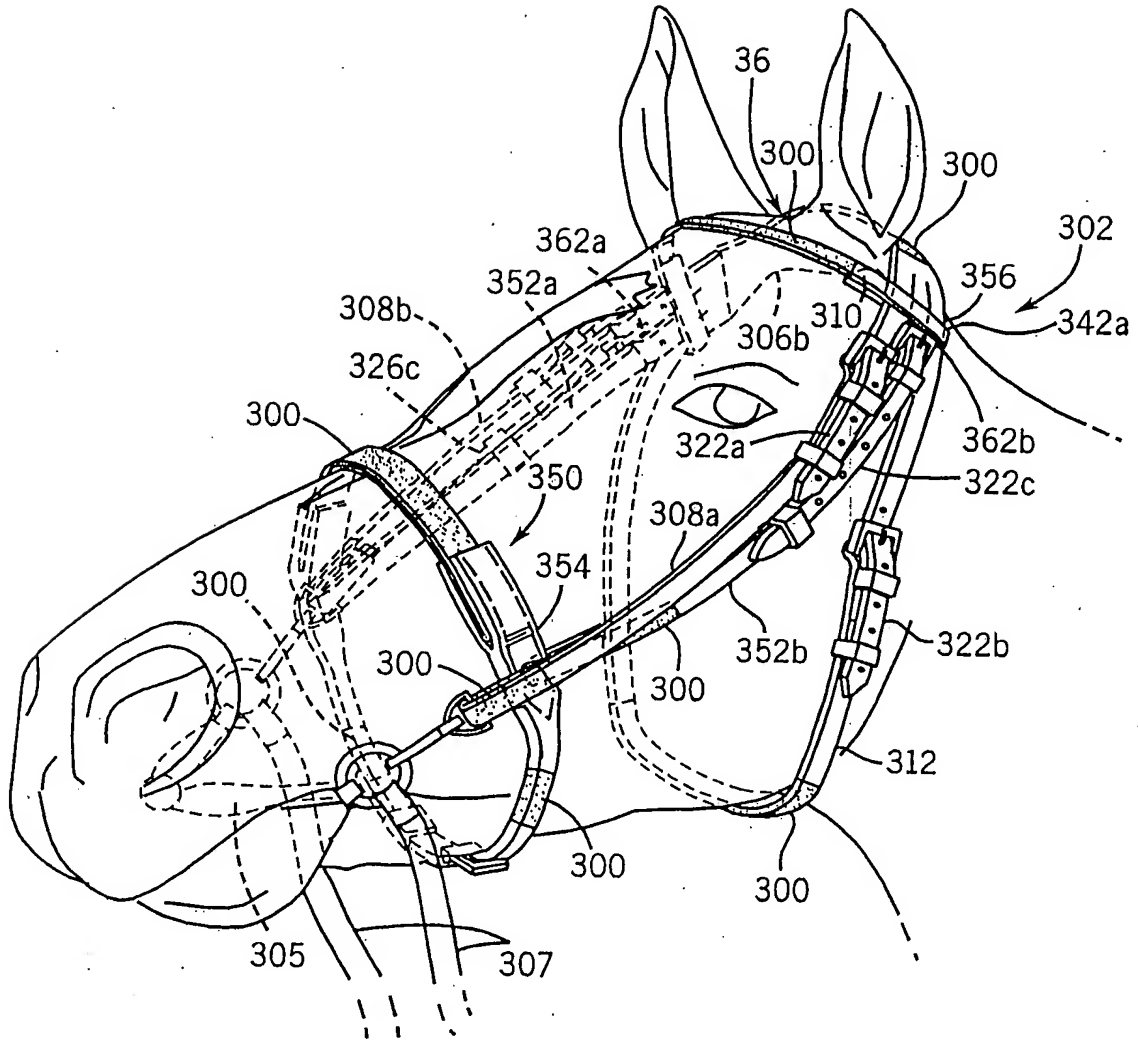
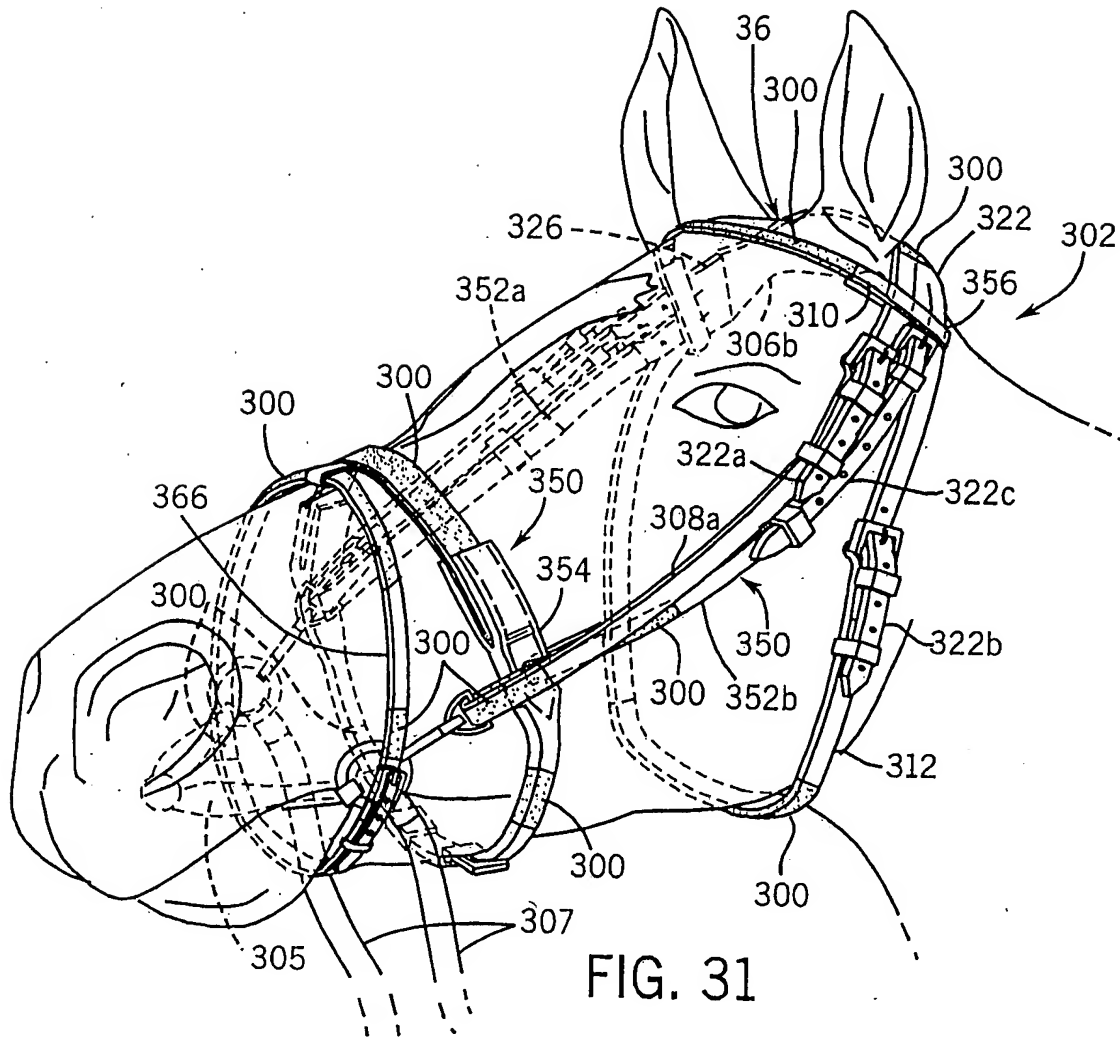
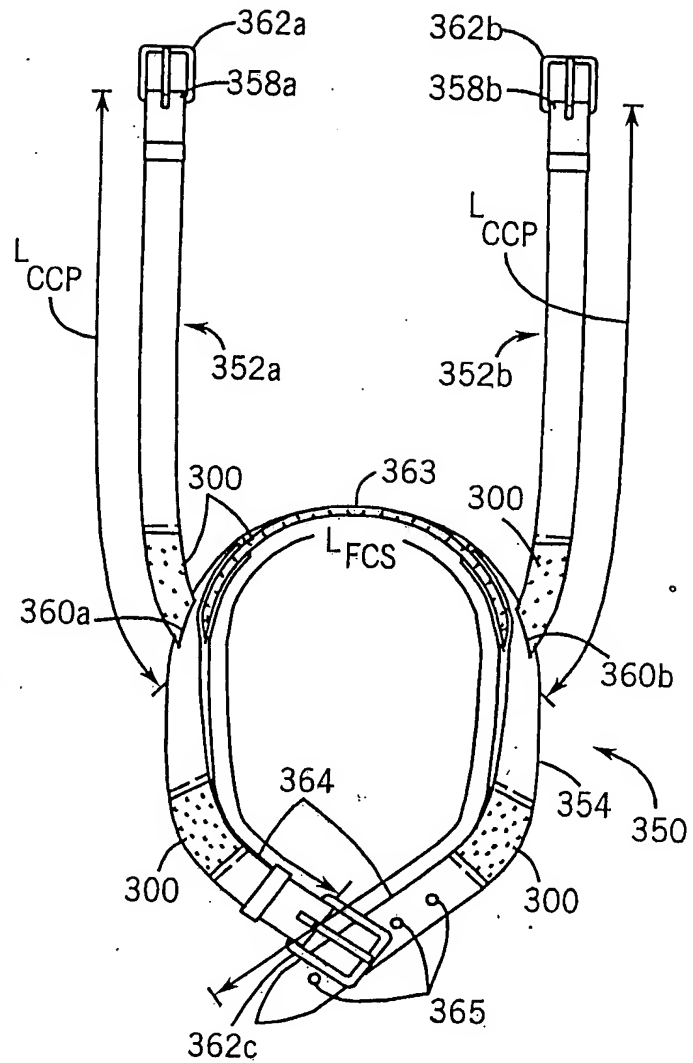
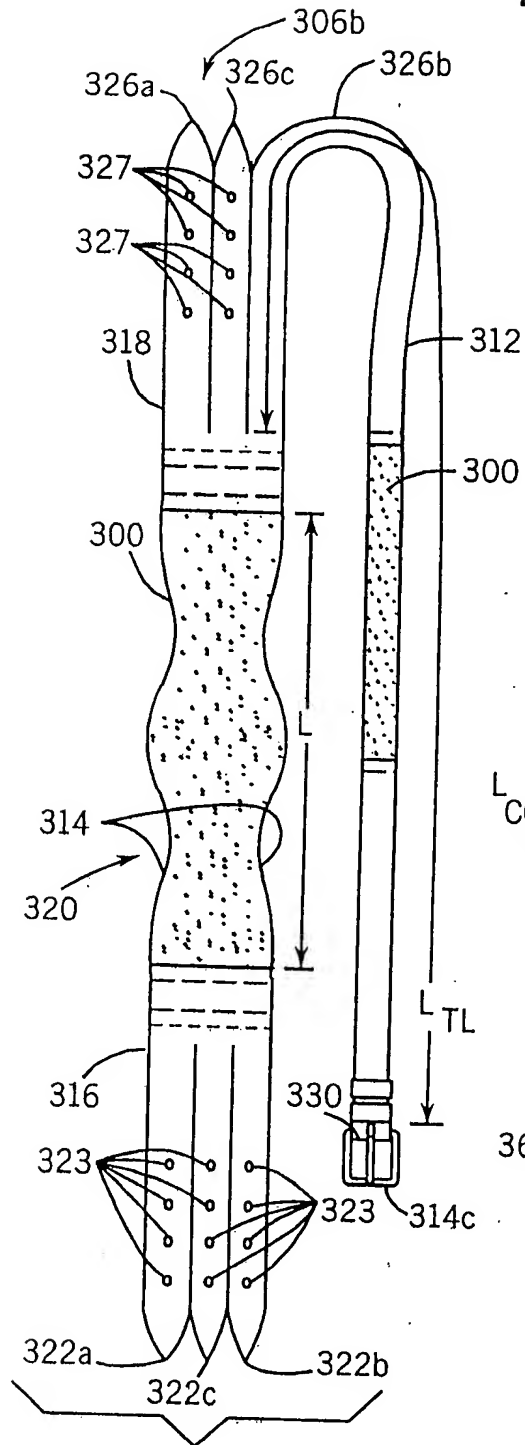
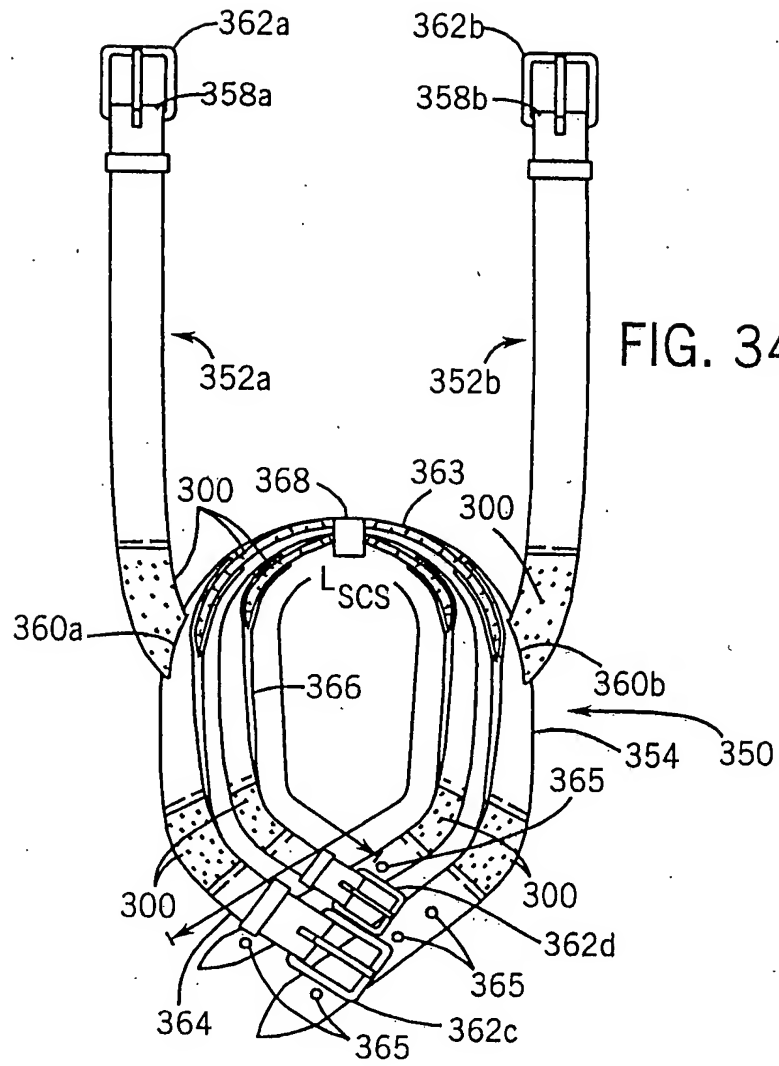
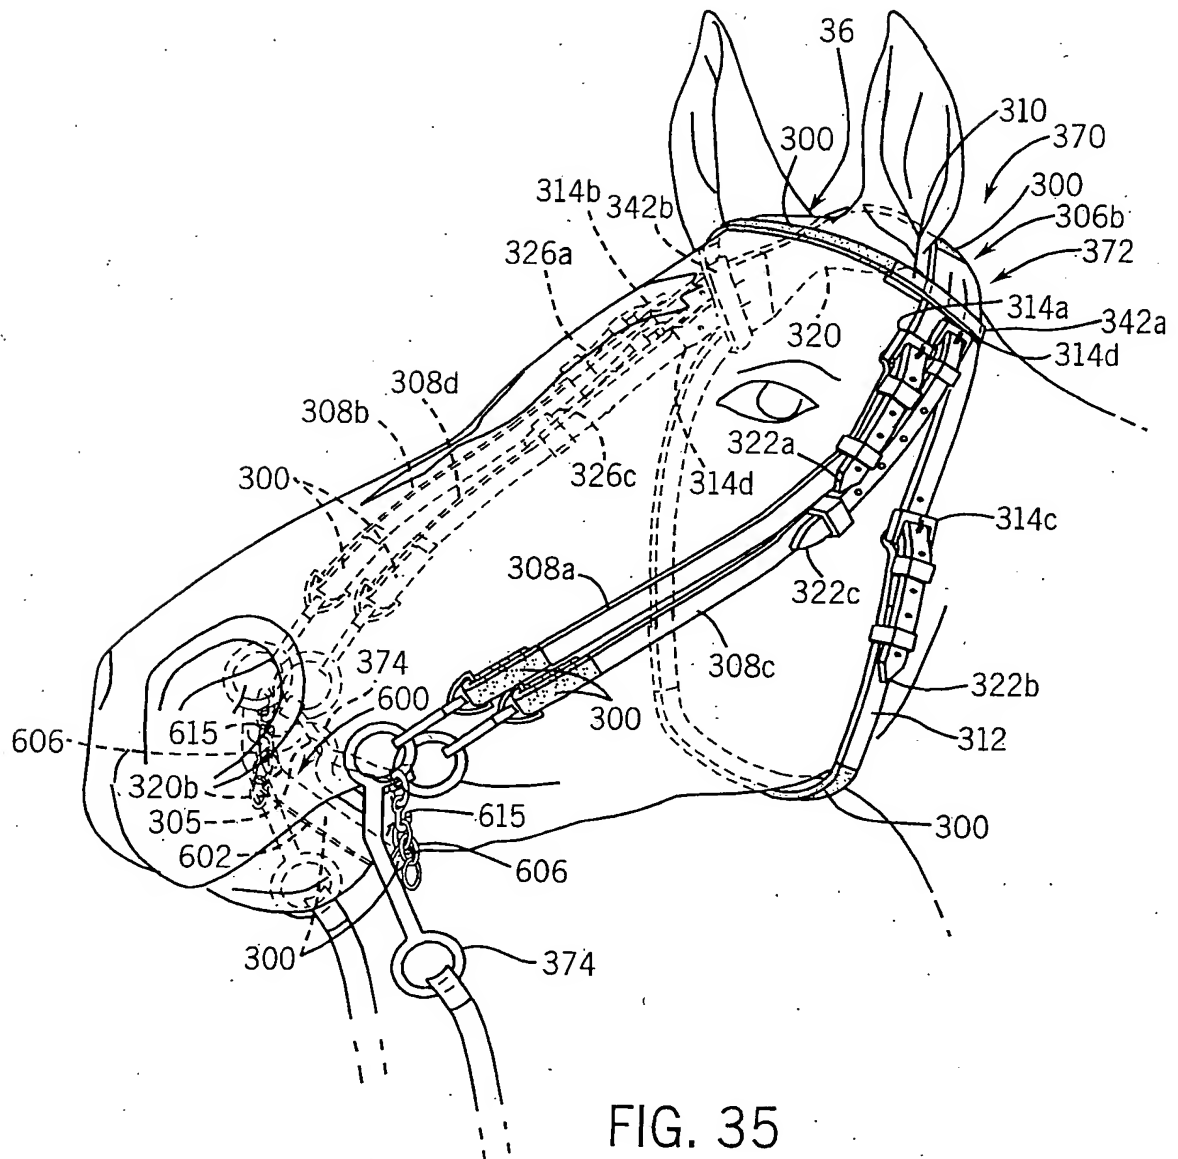


FIG. 30









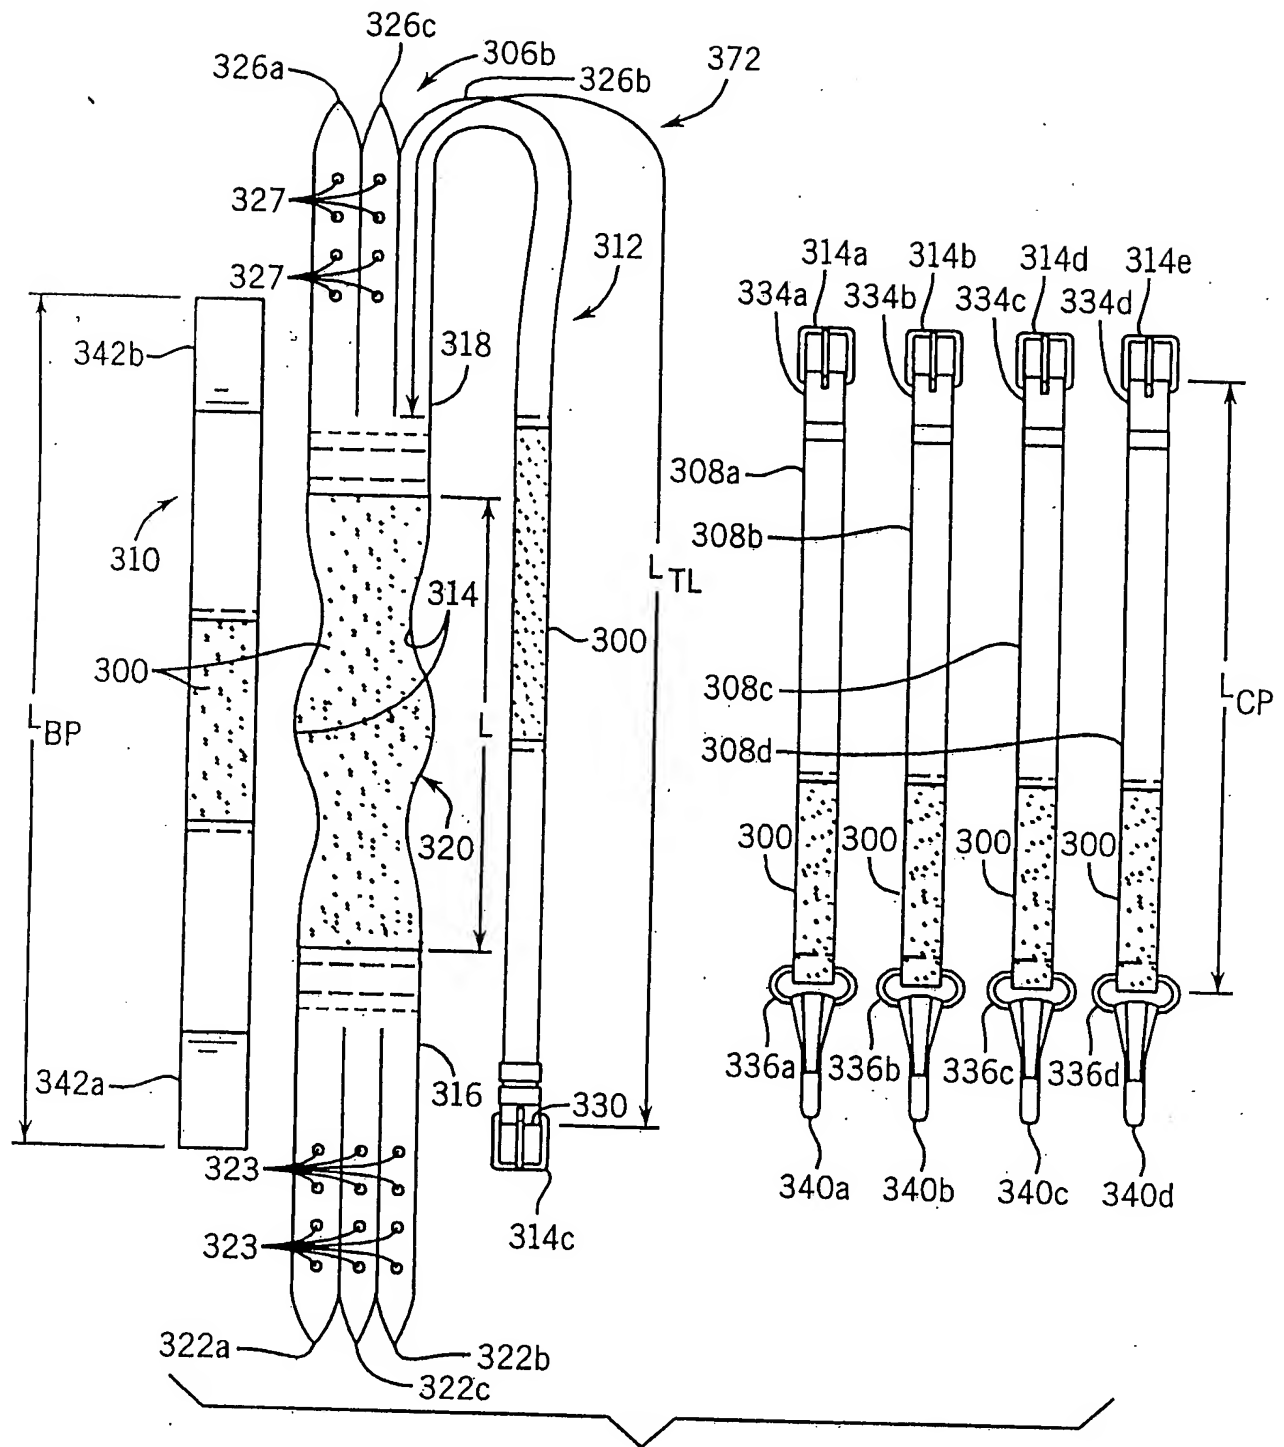


FIG. 36

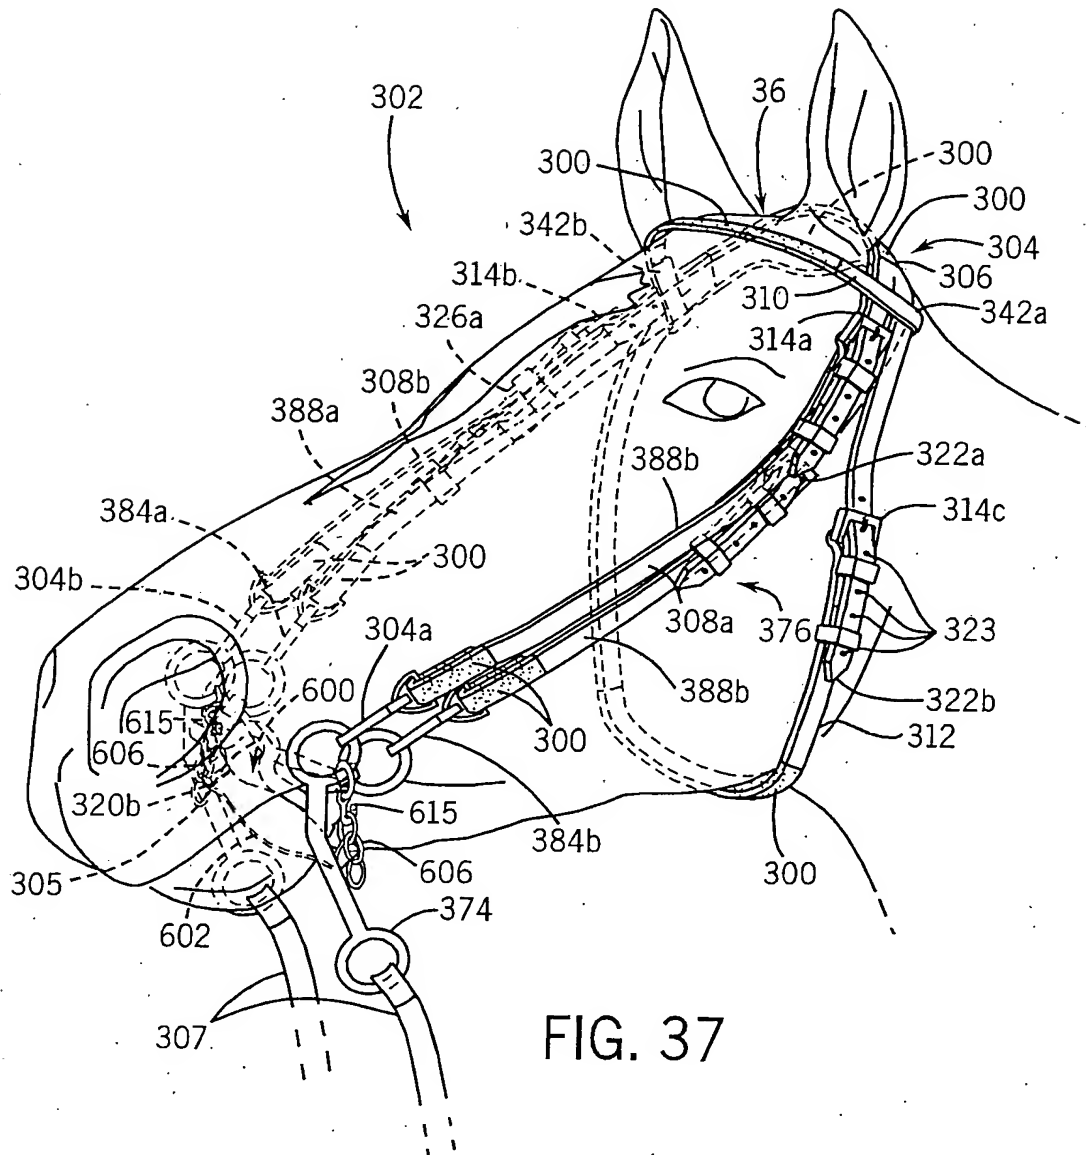


FIG. 37



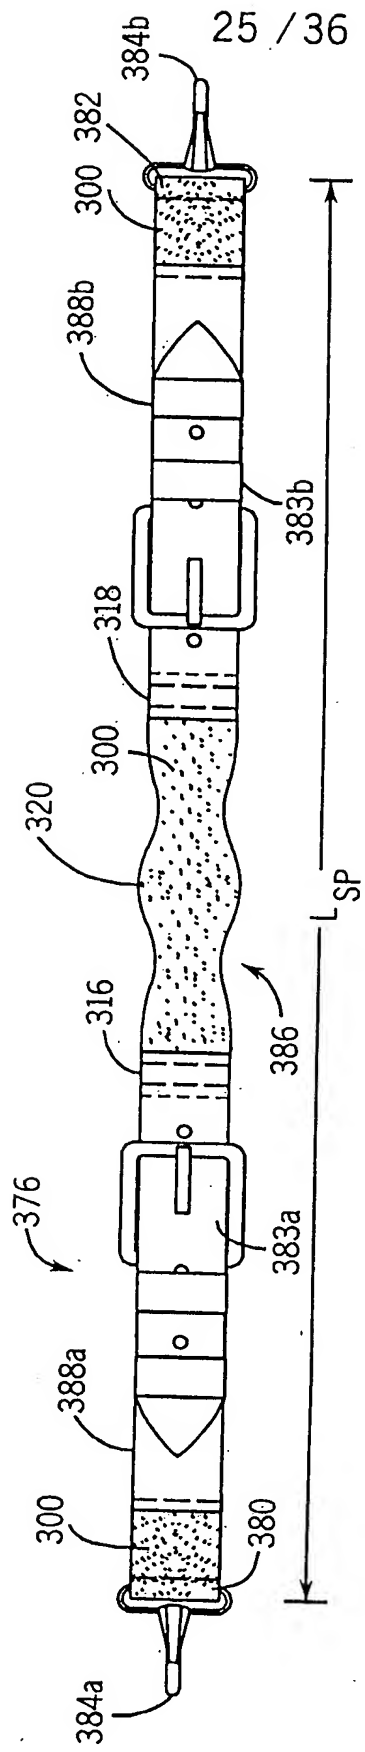


FIG. 38

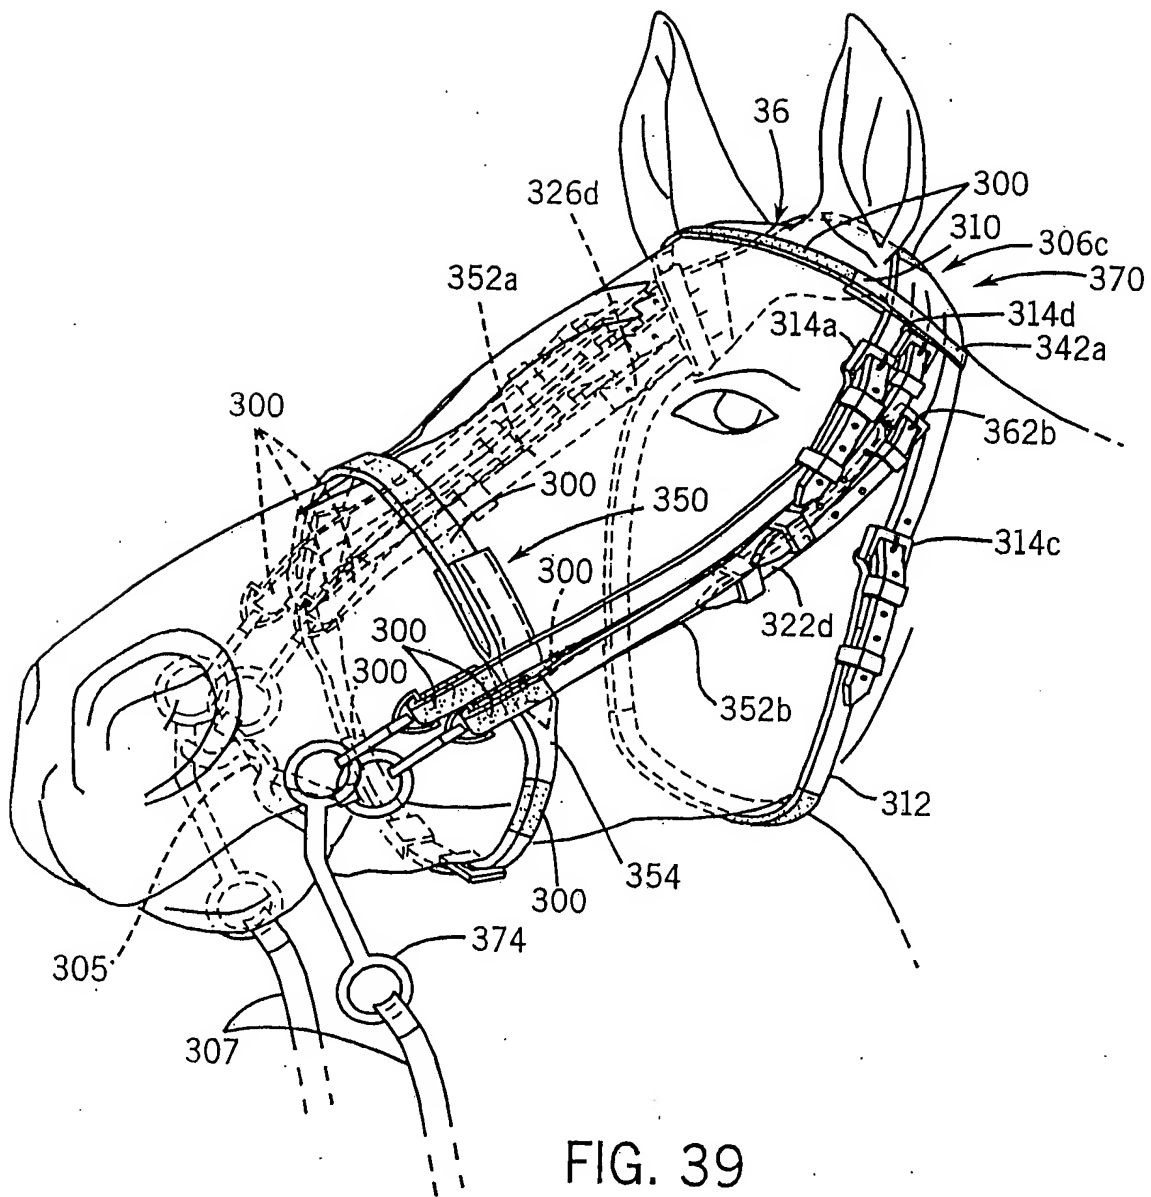


FIG. 39

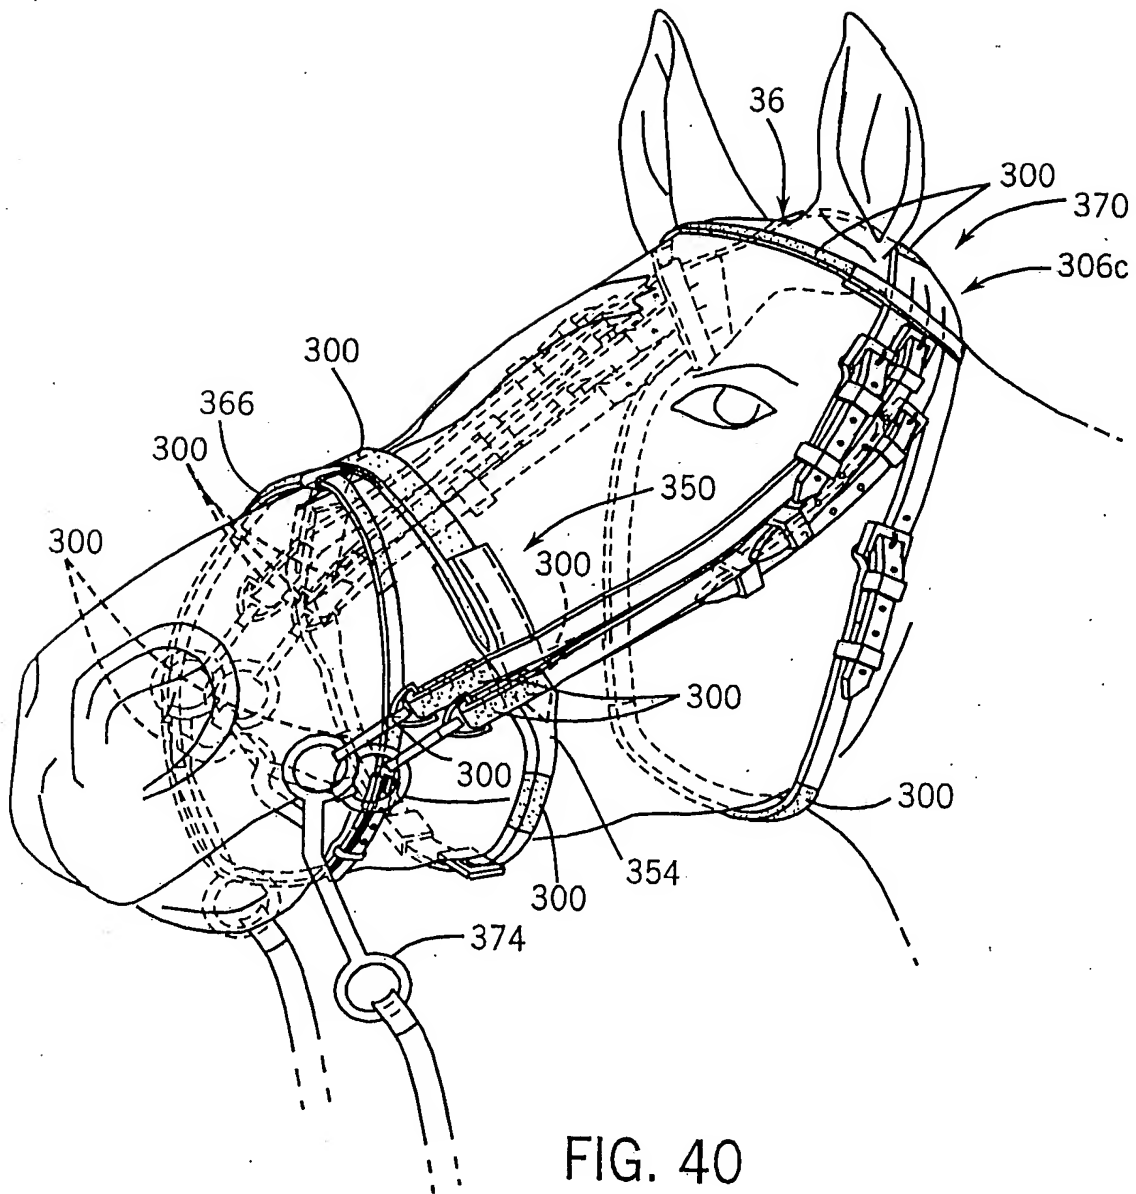


FIG. 40

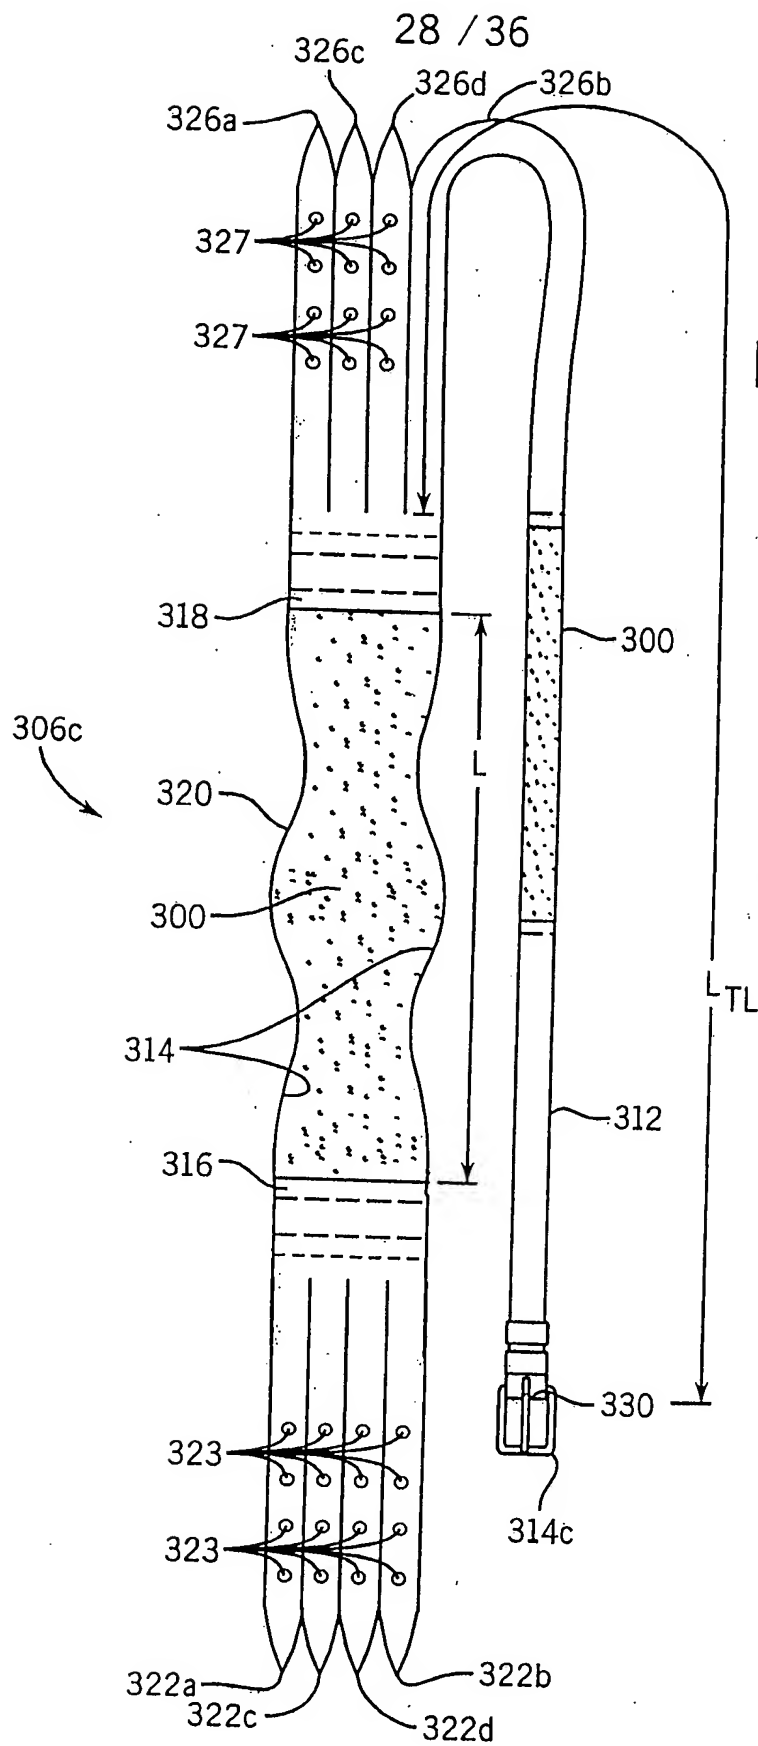


FIG. 41



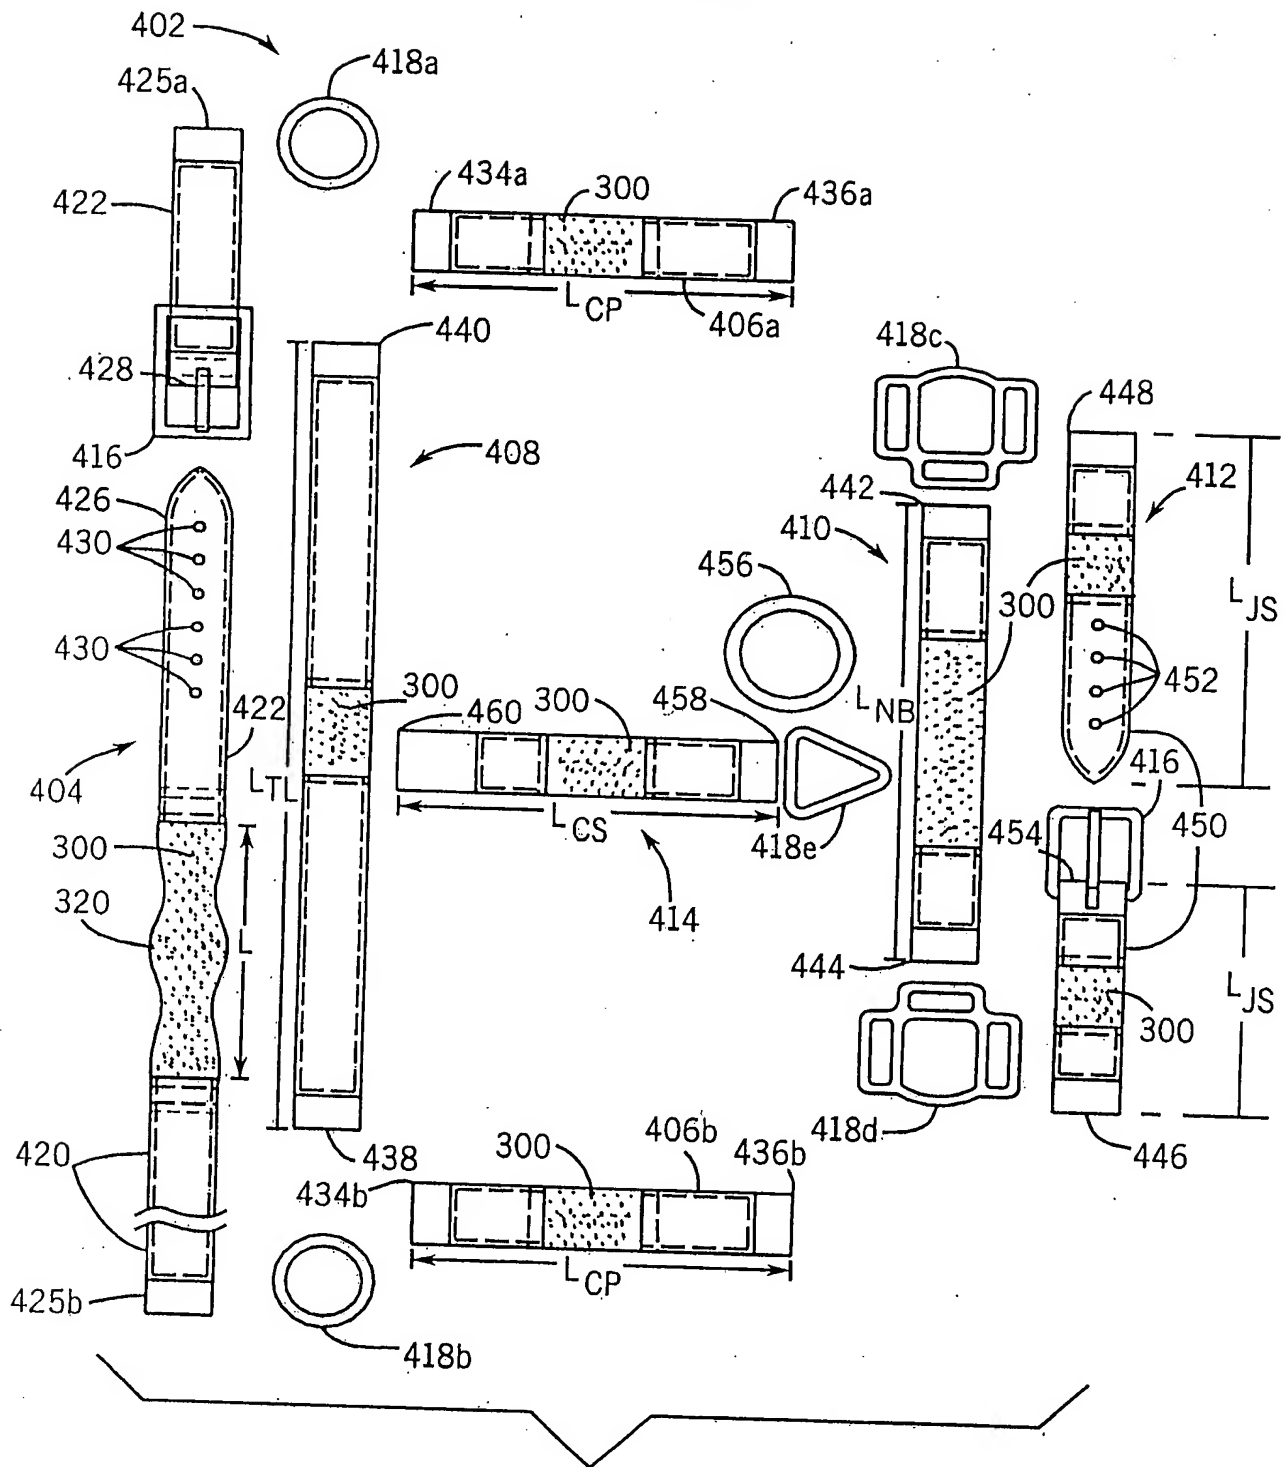


FIG. 43

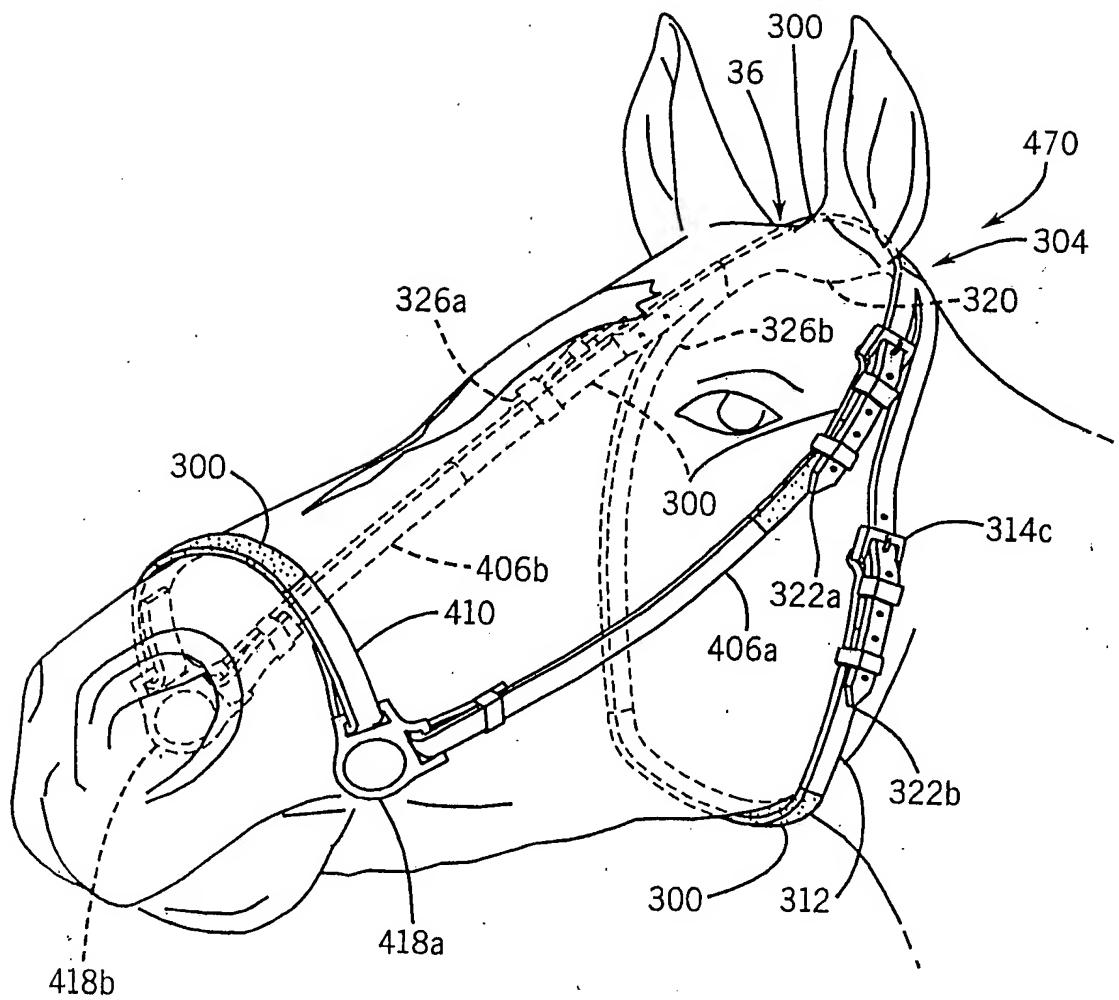


FIG. 44

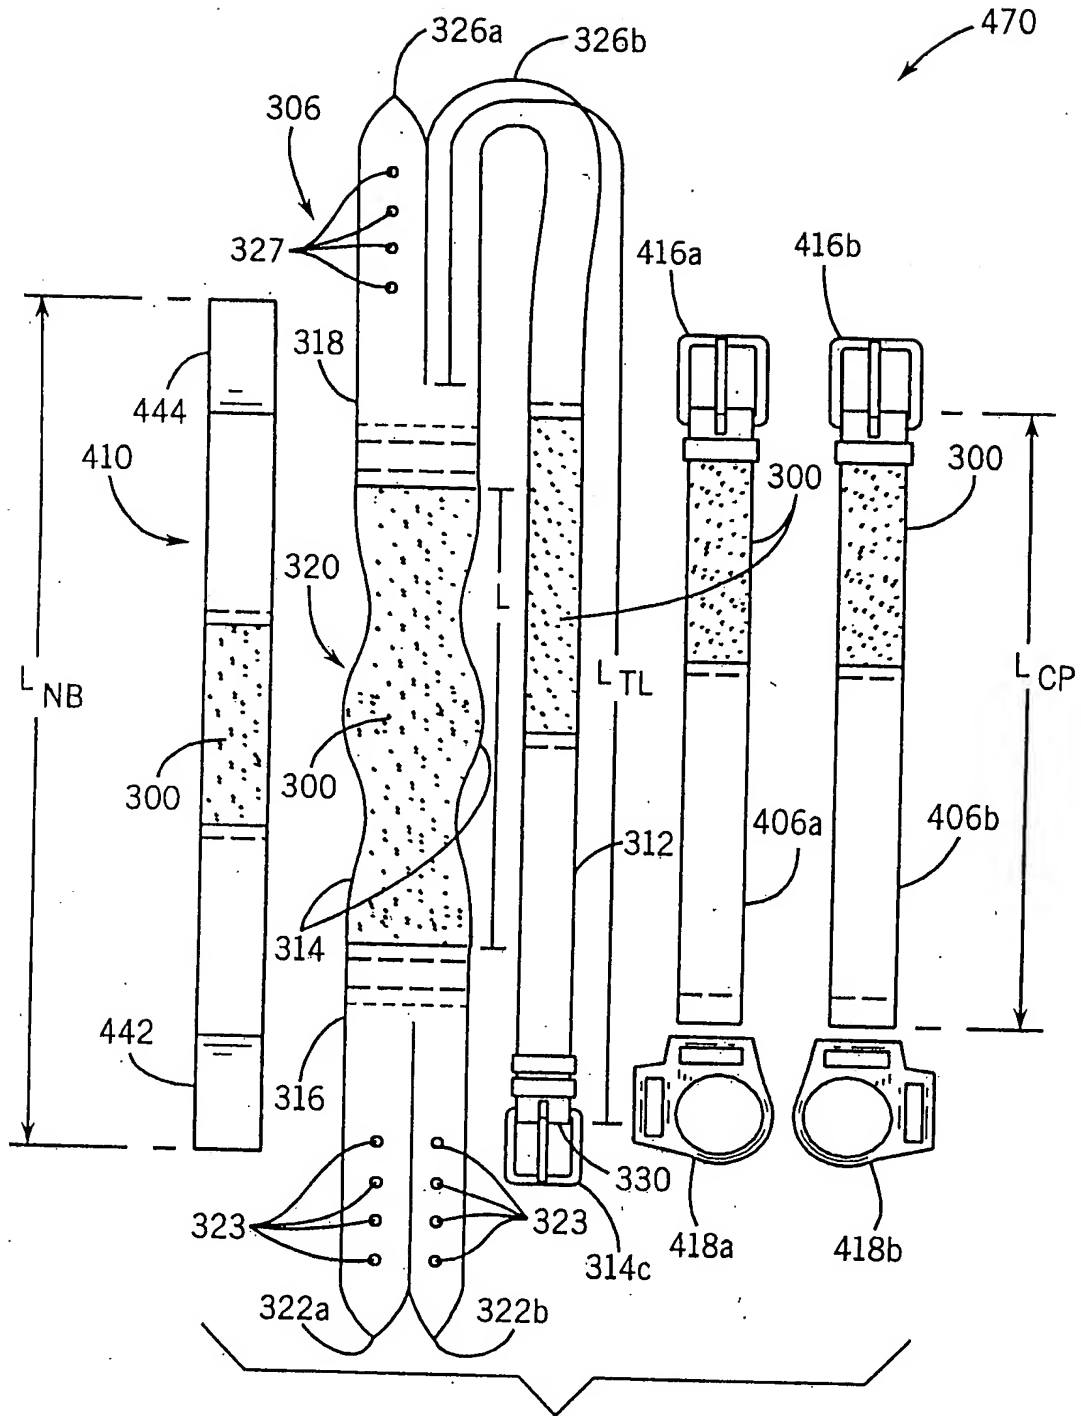


FIG. 45



